

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024618.D
 Acq On : 11 Feb 2022 21:24
 Operator : SY/MD
 Sample : VV0211WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK303

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	92209	90664	16.33%	2.105%
2	1.571	157	165	180	rVB	81379	90128	16.24%	2.092%
3	2.111	322	333	348	rBV	167059	239667	43.18%	5.564%
4	3.899	879	889	933	rBV	41982	155111	27.94%	3.601%
5	4.352	1014	1030	1060	rBV	94469	237415	42.77%	5.512%
6	5.050	1231	1247	1281	rBV2	224412	555089	100.00%	12.887%
7	5.619	1412	1424	1449	rBV	139694	285215	51.38%	6.621%
8	5.911	1506	1515	1530	rBV4	5603	11665	2.10%	0.271%
9	6.069	1552	1564	1591	rBV2	124158	256745	46.25%	5.960%
10	6.985	1839	1849	1874	rBV	63387	119369	21.50%	2.771%
11	7.317	1940	1952	1972	rBV	285220	501010	90.26%	11.631%
12	7.400	1973	1978	1991	rVB5	3821	6077	1.09%	0.141%
13	7.622	2038	2047	2067	rBV	35172	64131	11.55%	1.489%
14	8.088	2182	2192	2232	rBV	223000	438396	78.98%	10.178%
15	8.850	2419	2429	2459	rBV	228898	371728	66.97%	8.630%
16	10.214	2843	2853	2873	rBV	68903	109045	19.64%	2.532%
17	11.249	3164	3175	3198	rBV	246845	383857	69.15%	8.911%
18	11.622	3280	3291	3314	rBV	238867	379554	68.38%	8.812%
19	12.249	3472	3486	3495	rBV	3510	5650	1.02%	0.131%
20	14.040	4032	4043	4052	rVB	4177	6958	1.25%	0.162%




Sum of corrected areas: 4307474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024618.D
Acq On : 11 Feb 2022 21:24
Operator : SY/MD
Sample : VV0211WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

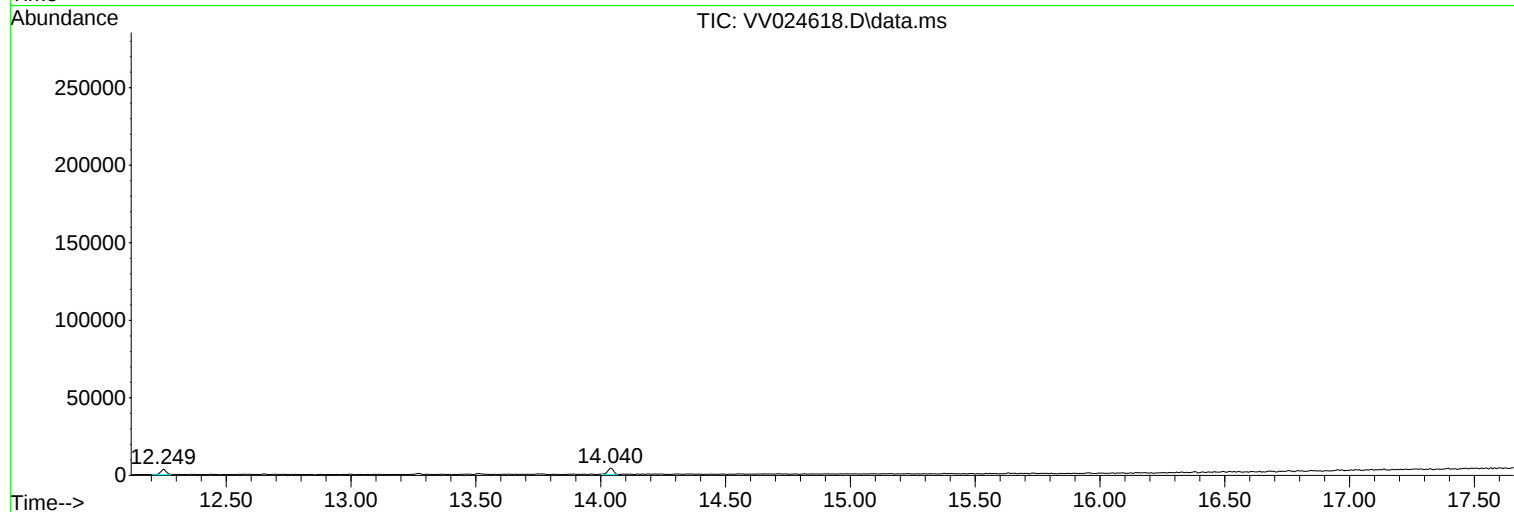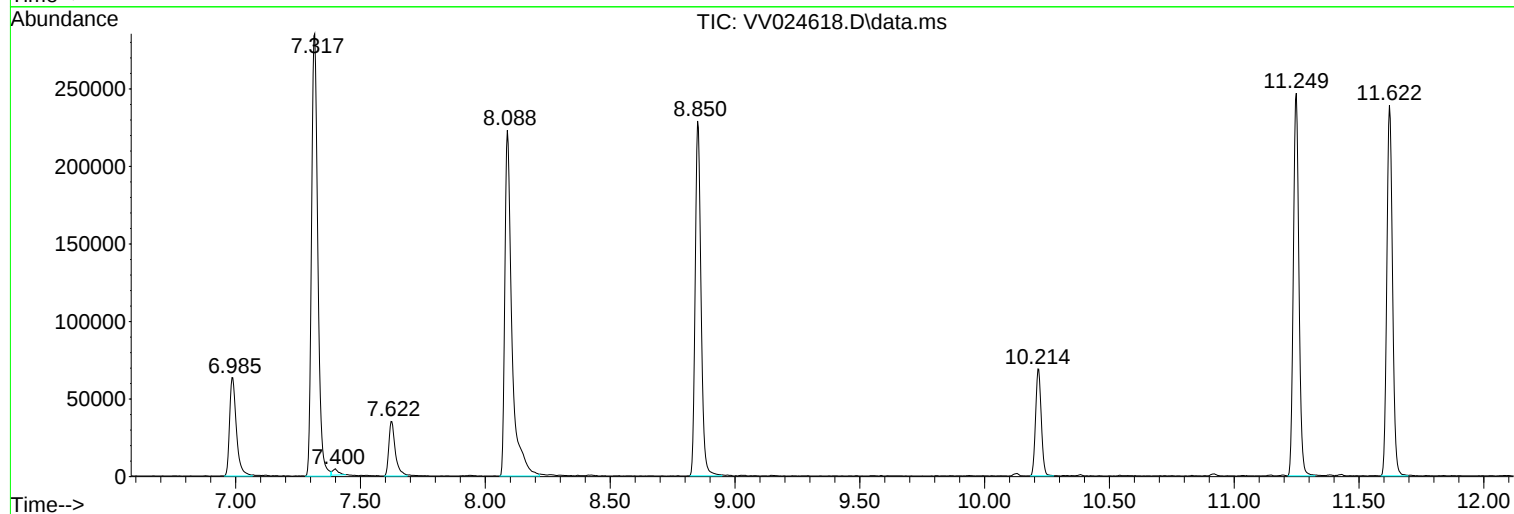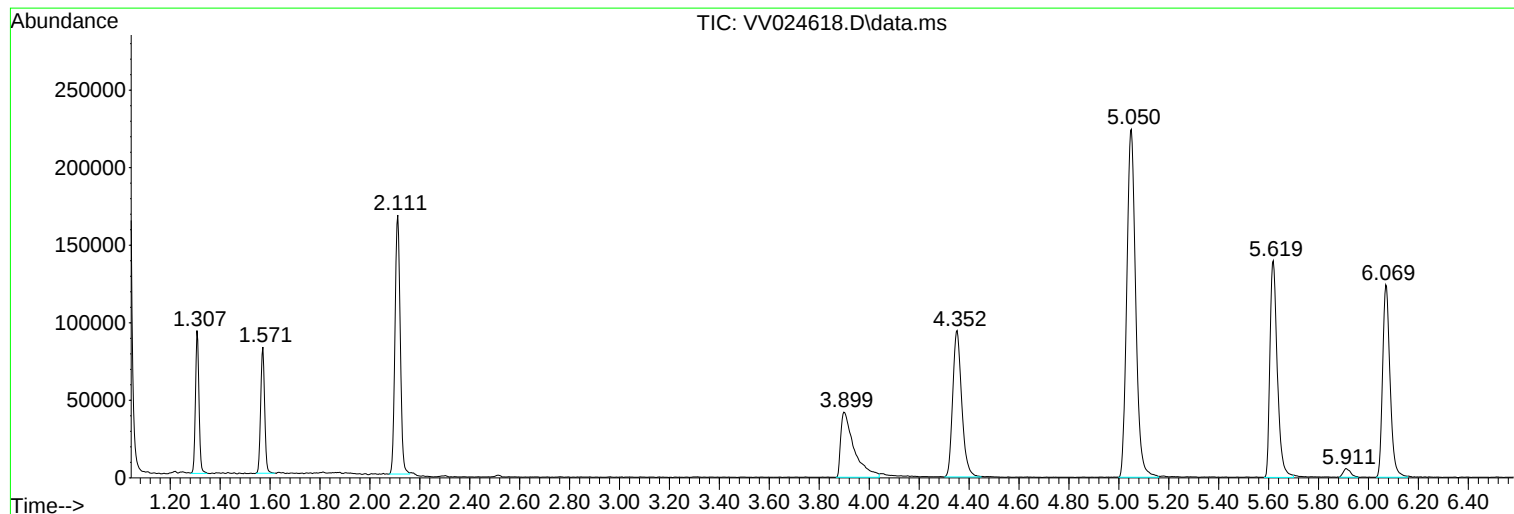

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024618.D
Acq On : 11 Feb 2022 21:24
Operator : SY/MD
Sample : VV0211WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024618.D
Acq On : 11 Feb 2022 21:24
Operator : SY/MD
Sample : VV0211WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc