

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024620.D
 Acq On : 11 Feb 2022 22:34
 Operator : SY/MD
 Sample : N1512-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	63642	65740	14.82%	1.724%
2	1.571	157	165	175	rBV	58204	66179	14.92%	1.735%
3	2.111	321	333	348	rBV	119762	175140	39.48%	4.592%
4	2.166	348	350	367	rVB6	2462	4456	1.00%	0.117%
5	3.899	880	889	924	rBV	39611	140713	31.72%	3.689%
6	4.352	1013	1030	1051	rBV2	76120	191654	43.20%	5.025%
7	5.050	1232	1247	1275	rBV2	179307	443604	100.00%	11.631%
8	5.619	1412	1424	1444	rBV	138929	277022	62.45%	7.263%
9	5.912	1505	1515	1530	rVB4	5925	13025	2.94%	0.342%
10	6.072	1552	1565	1591	rBV	101043	212479	47.90%	5.571%
11	6.568	1708	1719	1736	rBV4	12545	27133	6.12%	0.711%
12	6.989	1840	1850	1872	rBV	51189	95454	21.52%	2.503%
13	7.137	1883	1896	1915	rVB2	53076	100848	22.73%	2.644%
14	7.317	1940	1952	1972	rBV	218814	381958	86.10%	10.015%
15	7.404	1975	1979	1996	rVB2	3817	5718	1.29%	0.150%
16	7.625	2039	2048	2069	rBV	28121	51470	11.60%	1.350%
17	8.088	2182	2192	2230	rBV	193157	390169	87.95%	10.230%
18	8.850	2419	2429	2453	rBV	220264	365975	82.50%	9.596%
19	9.127	2506	2515	2525	rBV3	7122	11908	2.68%	0.312%
20	10.214	2840	2853	2869	rBV	57784	91153	20.55%	2.390%
21	11.059	3109	3116	3125	rBV3	3107	4728	1.07%	0.124%
22	11.246	3163	3174	3196	rBV	248392	375354	84.61%	9.842%
23	11.532	3254	3263	3278	rBV3	7081	13286	3.00%	0.348%
24	11.622	3280	3291	3313	rVB	195132	308737	69.60%	8.095%




Sum of corrected areas: 3813903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024620.D
Acq On : 11 Feb 2022 22:34
Operator : SY/MD
Sample : N1512-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

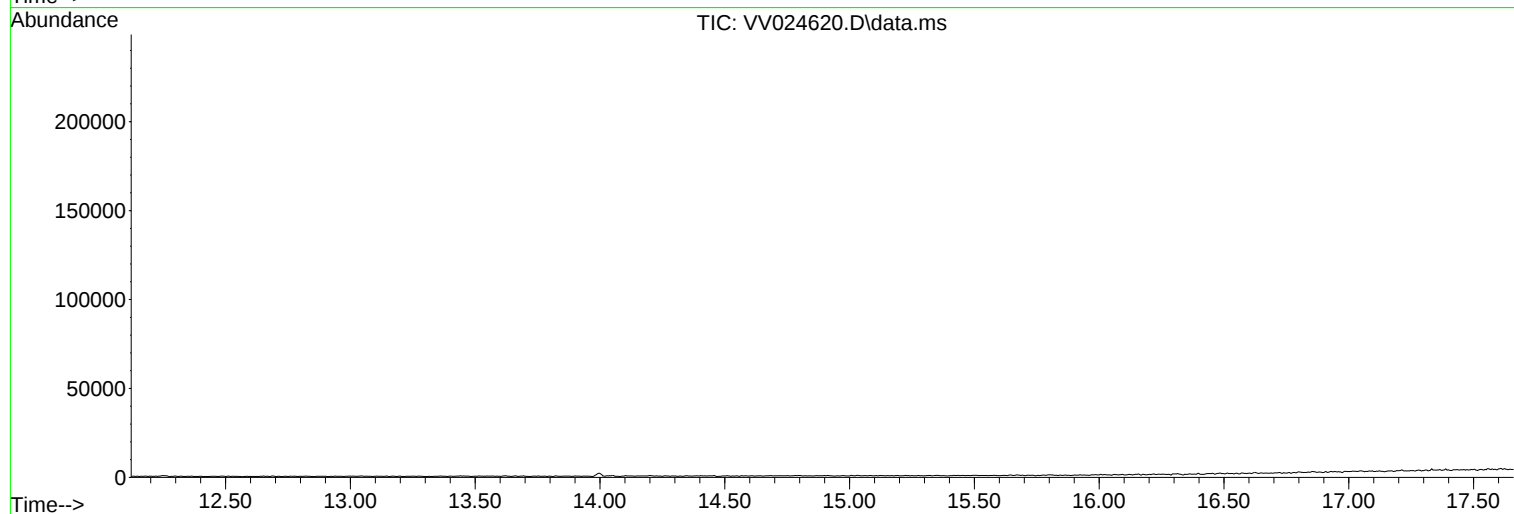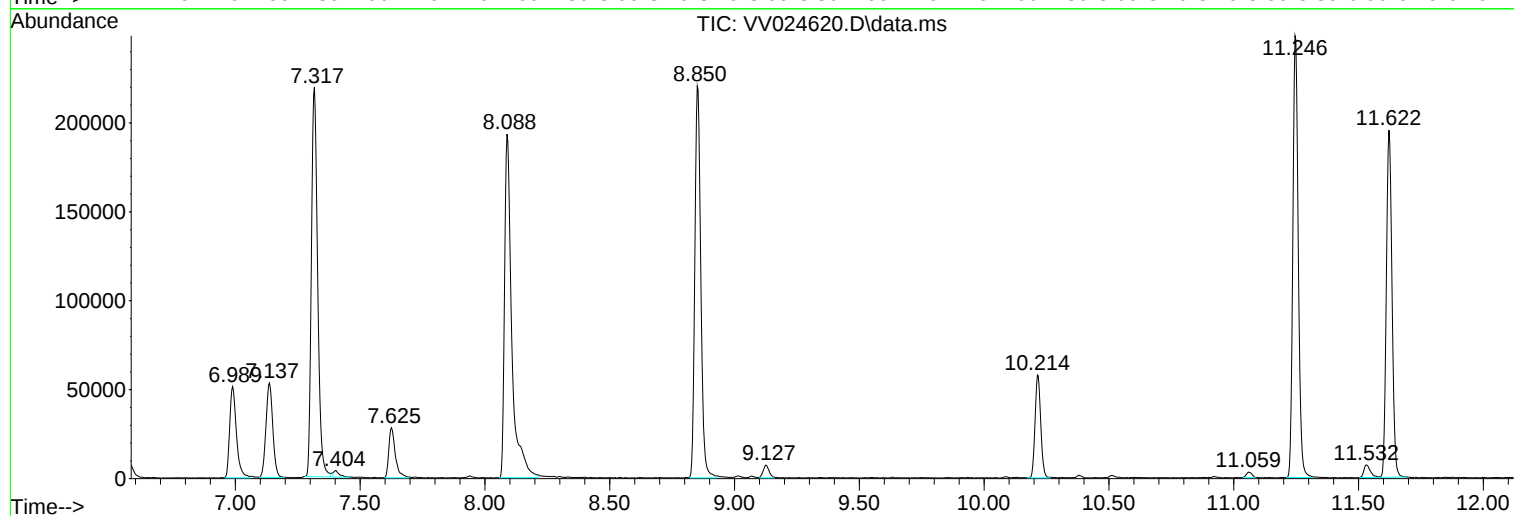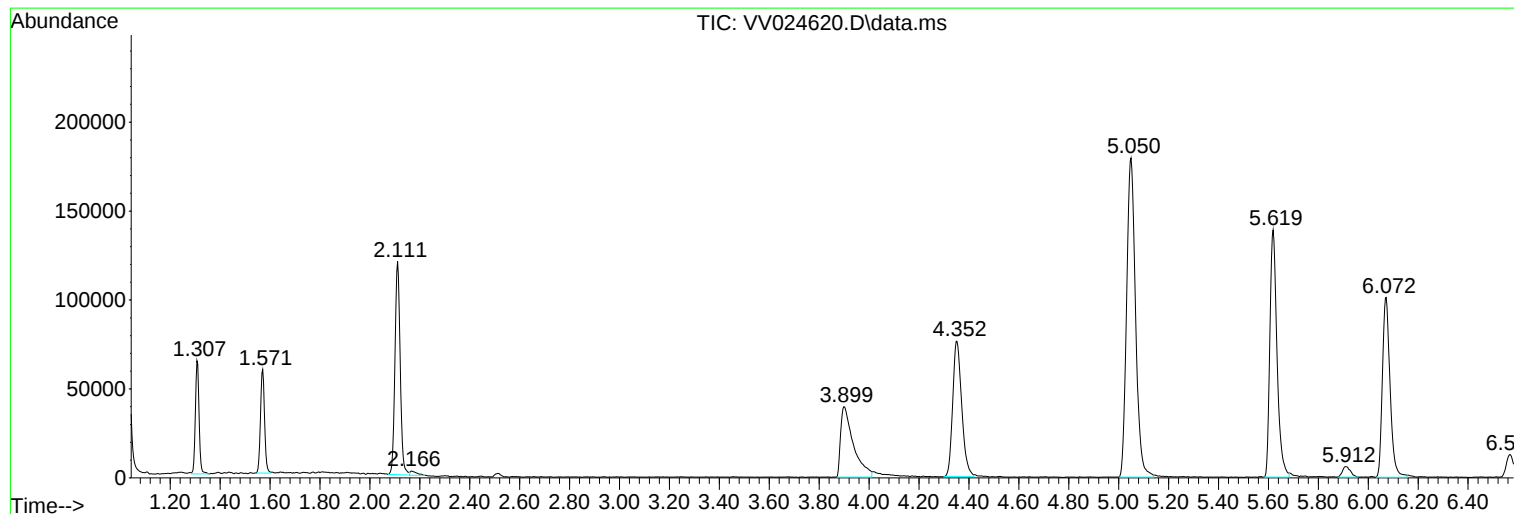

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024620.D
Acq On : 11 Feb 2022 22:34
Operator : SY/MD
Sample : N1512-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Furan, tetrahydro-2,2,4,4-t... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.137	1.82 ug/L	100848	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Furan, tetrahydro-2,2,4,4-tetram...	128	C8H16O	003358-28-9	53
2			4-Piperidinone, 1-methyl-	113	C6H11NO	001445-73-4	50
3			Furan, tetrahydro-2,2,5,5-tetram...	128	C8H16O	015045-43-9	50
4			1,3,5-Triazine-2,4(1H,3H)-dione	113	C3H3N3O2	000071-33-0	43
5			Furan, tetrahydro-2,2,4,4-tetram...	128	C8H16O	003358-28-9	42

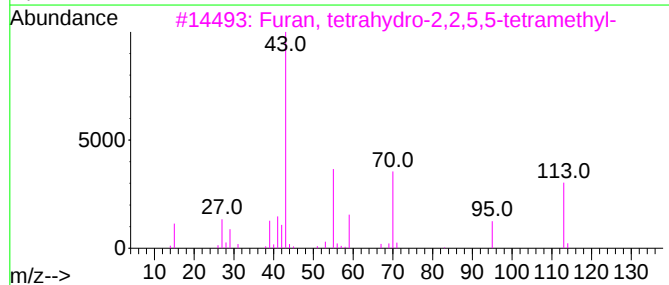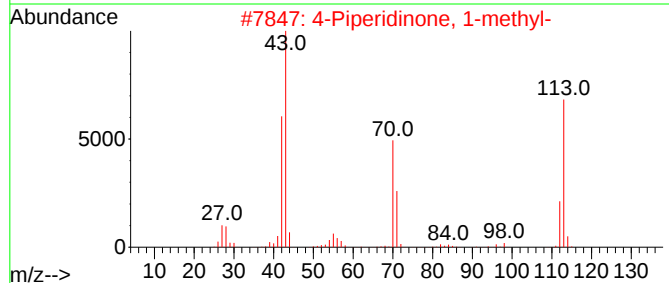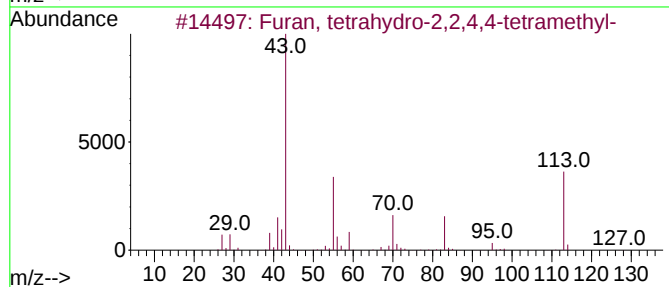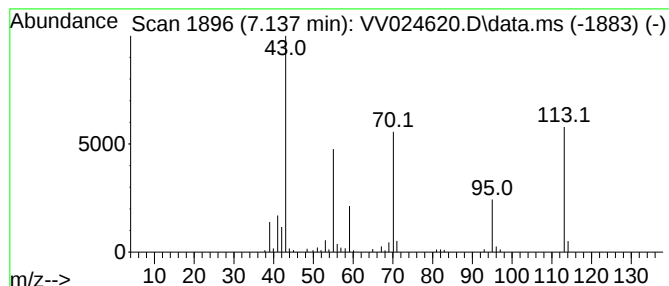

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024620.D
Acq On : 11 Feb 2022 22:34
Operator : SY/MD
Sample : N1512-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Furan, tetrahyd...	7.137	1.8	ug/L	100848	1	5.619	277022	5.0