

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024621.D
 Acq On : 11 Feb 2022 22:58
 Operator : SY/MD
 Sample : N1512-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	64039	64033	14.35%	1.599%
2	1.571	157	165	176	rBV	61390	68785	15.42%	1.718%
3	1.757	214	223	232	rBV5	2418	4491	1.01%	0.112%
4	2.111	322	333	353	rVB	121220	178784	40.07%	4.466%
5	3.902	878	890	938	rBV	40804	160732	36.03%	4.015%
6	4.352	1014	1030	1057	rBV	76207	195583	43.84%	4.885%
7	5.050	1228	1247	1278	rBV2	178766	446147	100.00%	11.143%
8	5.619	1413	1424	1453	rBV	136851	278596	62.44%	6.959%
9	5.915	1504	1516	1533	rVB7	4830	10767	2.41%	0.269%
10	6.069	1552	1564	1584	rBV	100913	209726	47.01%	5.238%
11	6.989	1840	1850	1869	rBV	51379	95486	21.40%	2.385%
12	7.317	1939	1952	1972	rBV	220751	388313	87.04%	9.699%
13	7.625	2039	2048	2068	rBV2	29247	52092	11.68%	1.301%
14	7.976	2146	2157	2178	rBV	169059	281571	63.11%	7.033%
15	8.088	2183	2192	2225	rBV	204054	395812	88.72%	9.886%
16	8.853	2418	2430	2452	rBV	225599	370632	83.07%	9.257%
17	10.217	2843	2854	2866	rBV	62061	97174	21.78%	2.427%
18	11.249	3164	3175	3197	rBV	247559	384400	86.16%	9.601%
19	11.535	3254	3264	3274	rBV6	4929	8936	2.00%	0.223%
20	11.622	3279	3291	3311	rVV	199563	311600	69.84%	7.783%




Sum of corrected areas: 4003660

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024621.D
Acq On : 11 Feb 2022 22:58
Operator : SY/MD
Sample : N1512-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

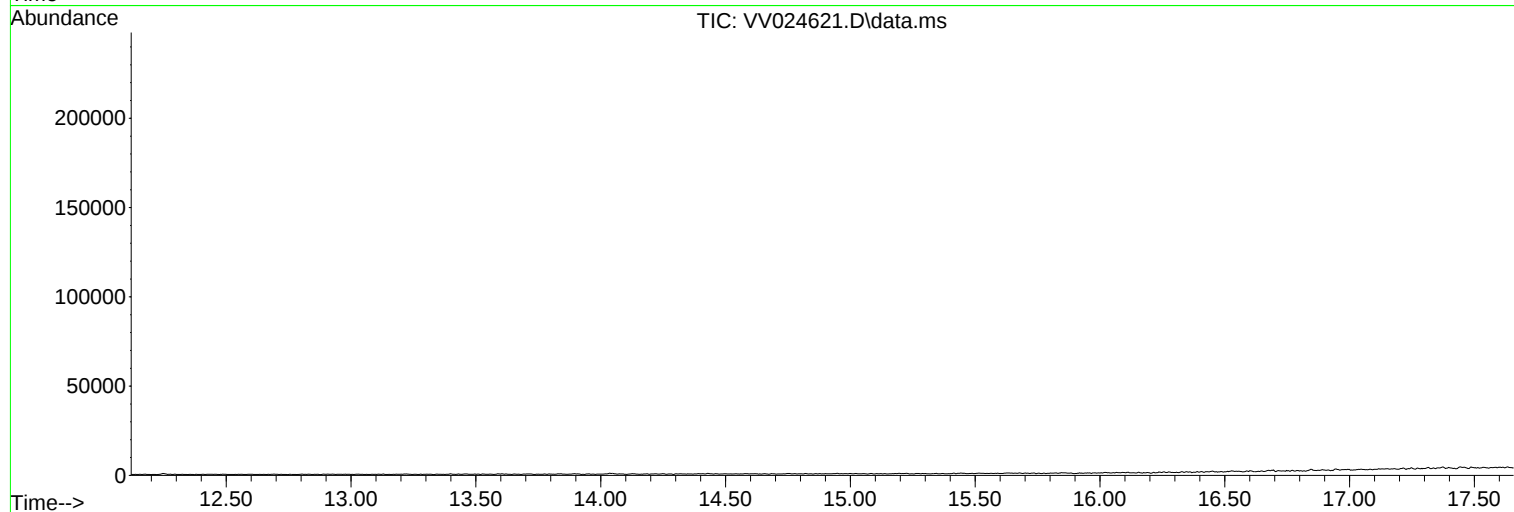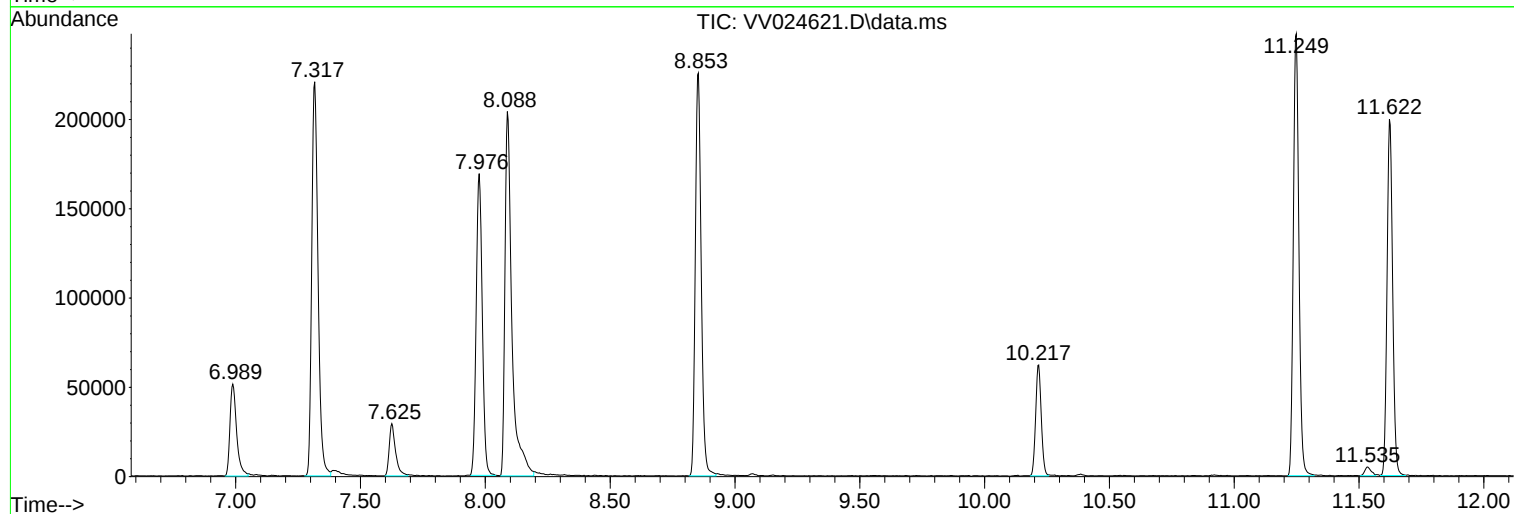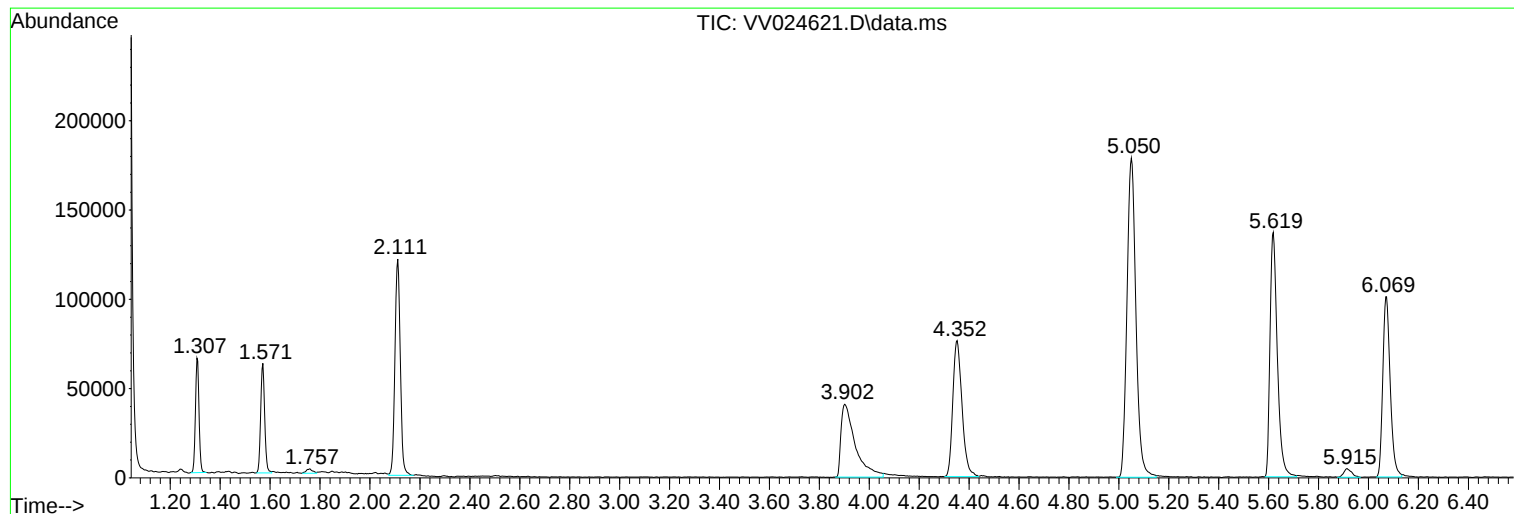

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024621.D
Acq On : 11 Feb 2022 22:58
Operator : SY/MD
Sample : N1512-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024621.D
Acq On : 11 Feb 2022 22:58
Operator : SY/MD
Sample : N1512-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
