

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024622.D
 Acq On : 11 Feb 2022 23:21
 Operator : SY/MD
 Sample : N1512-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	45	51	57	rBV	9448	8890	2.11%	0.254%
2	1.243	58	63	71	rVV2	4464	5005	1.19%	0.143%
3	1.307	74	83	97	rVB	62379	65011	15.47%	1.857%
4	1.571	157	165	176	rVB	57023	63192	15.03%	1.805%
5	2.111	322	333	353	rVB	111208	168102	39.99%	4.803%
6	3.912	874	893	936	rBV2	33656	149442	35.55%	4.270%
7	4.352	1014	1030	1058	rBV2	73819	185510	44.13%	5.300%
8	5.050	1230	1247	1274	rBV2	168242	420338	100.00%	12.009%
9	5.619	1413	1424	1451	rBV	136839	276165	65.70%	7.890%
10	5.908	1506	1514	1529	rBV4	3944	7797	1.85%	0.223%
11	6.069	1551	1564	1592	rBV	97611	203609	48.44%	5.817%
12	6.989	1838	1850	1877	rBV2	48028	91870	21.86%	2.625%
13	7.317	1941	1952	1970	rBV	206948	358067	85.19%	10.230%
14	7.400	1973	1978	1990	rVB3	2416	4655	1.11%	0.133%
15	7.625	2037	2048	2068	rBV	27839	50807	12.09%	1.452%
16	8.088	2180	2192	2227	rBV	191906	386495	91.95%	11.042%
17	8.850	2418	2429	2451	rBV	215627	358052	85.18%	10.230%
18	10.214	2843	2853	2874	rBV	59955	93871	22.33%	2.682%
19	11.249	3164	3175	3199	rBV	216100	333284	79.29%	9.522%
20	11.532	3255	3263	3274	rBV3	4418	7418	1.76%	0.212%
21	11.622	3281	3291	3311	rBV	167053	262548	62.46%	7.501%




Sum of corrected areas: 3500128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024622.D
Acq On : 11 Feb 2022 23:21
Operator : SY/MD
Sample : N1512-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

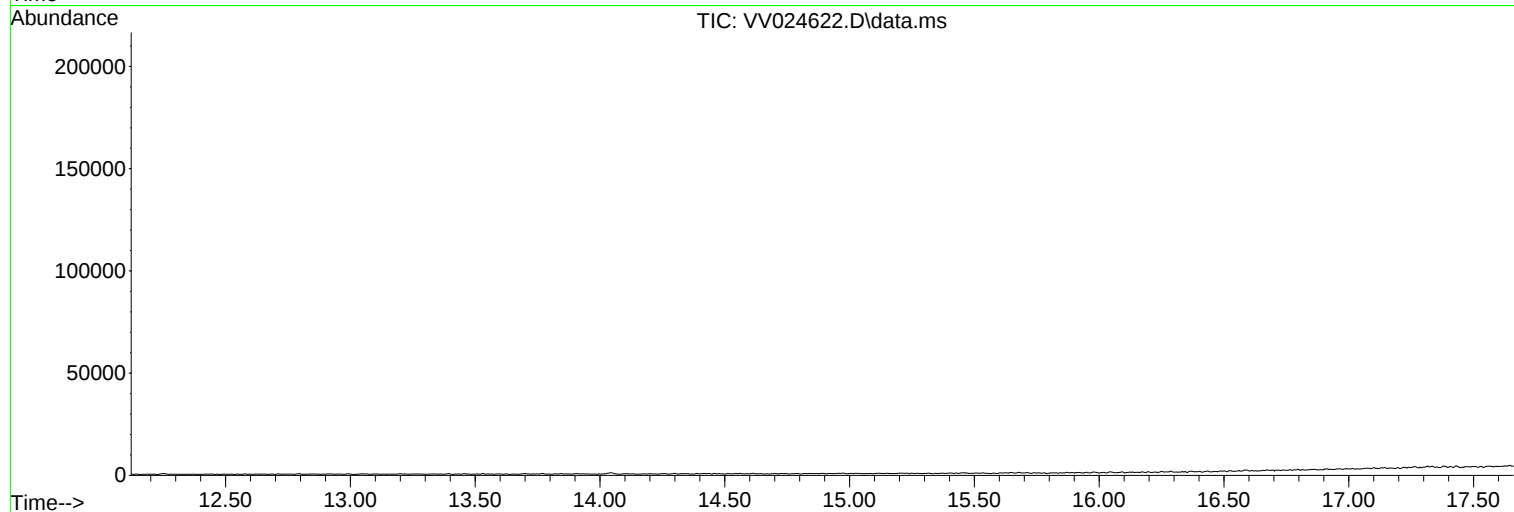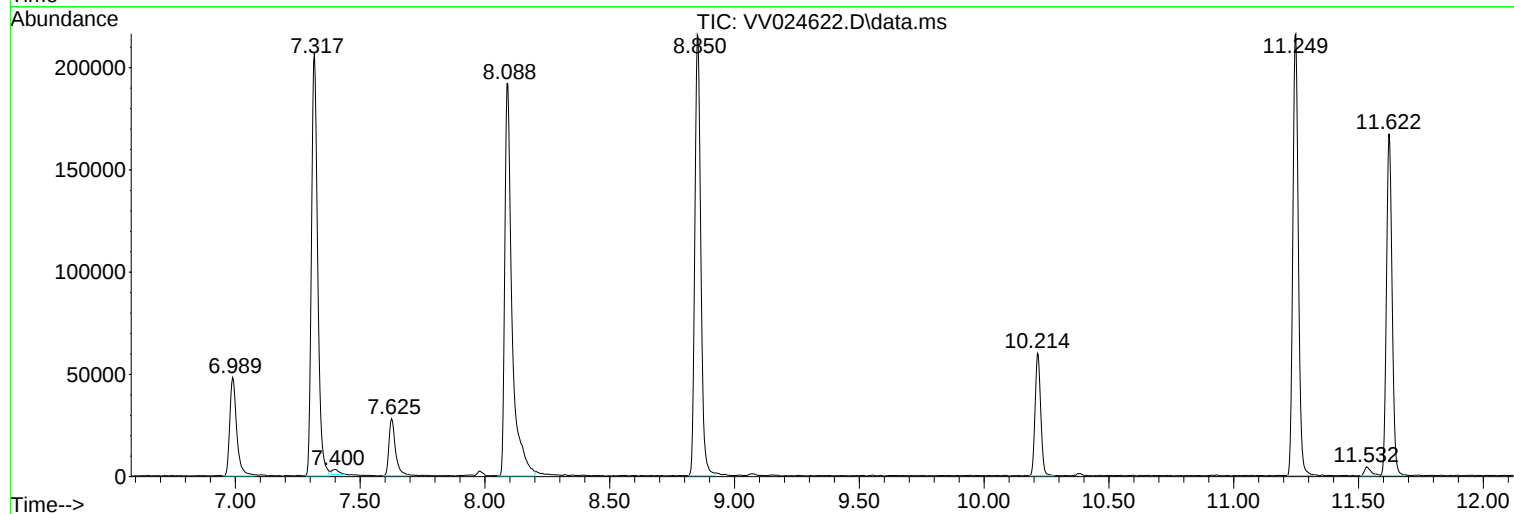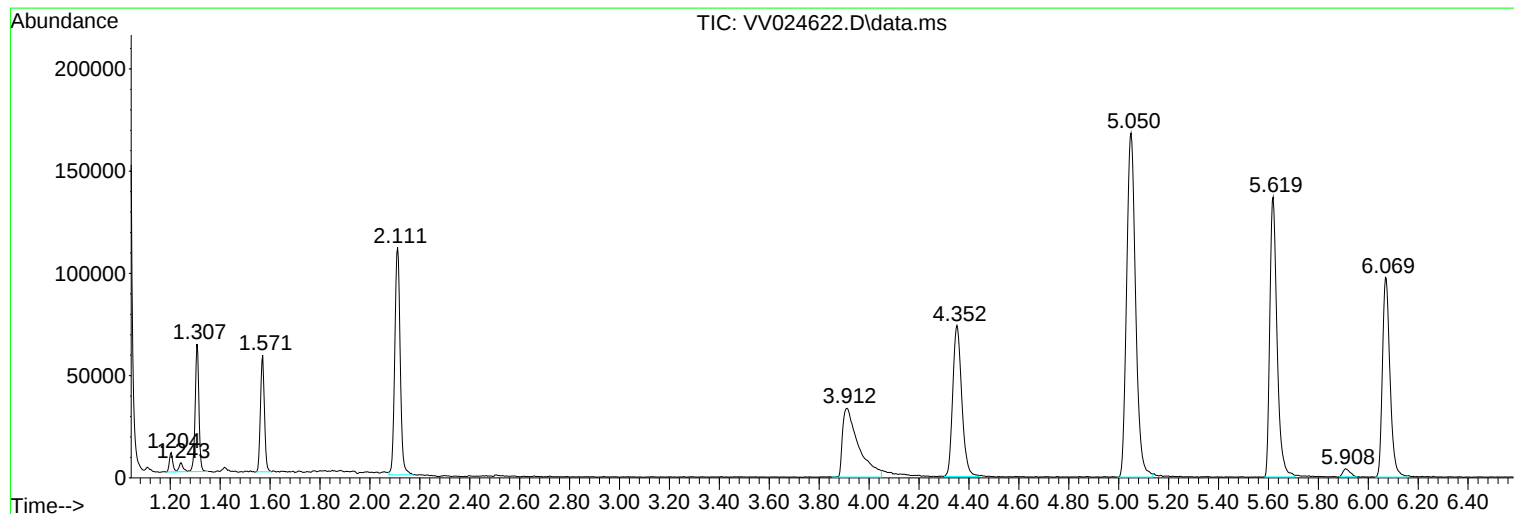

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024622.D
Acq On : 11 Feb 2022 23:21
Operator : SY/MD
Sample : N1512-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024622.D
Acq On : 11 Feb 2022 23:21
Operator : SY/MD
Sample : N1512-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
