

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024627.D
 Acq On : 12 Feb 2022 01:18
 Operator : SY/MD
 Sample : N1512-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	46	51	56	rBV	9601	8782	2.08%	0.245%
2	1.307	74	83	96	rVB	59432	64982	15.39%	1.810%
3	1.571	158	165	176	rBV	56802	62487	14.80%	1.741%
4	2.111	321	333	348	rBV	108463	158925	37.65%	4.427%
5	2.770	521	538	556	rBV2	21545	46927	11.12%	1.307%
6	3.905	877	891	930	rBV2	42558	168721	39.97%	4.700%
7	4.349	1013	1029	1064	rBV	72670	183425	43.45%	5.109%
8	5.050	1232	1247	1283	rBV2	170174	422105	100.00%	11.758%
9	5.619	1412	1424	1454	rBV	132321	268615	63.64%	7.482%
10	5.912	1505	1515	1527	rBV5	3807	7818	1.85%	0.218%
11	6.069	1552	1564	1596	rBV	97218	202954	48.08%	5.653%
12	6.989	1840	1850	1870	rBV	49778	91636	21.71%	2.553%
13	7.317	1941	1952	1972	rBV	205753	361487	85.64%	10.069%
14	7.625	2038	2048	2065	rBV2	26799	49290	11.68%	1.373%
15	8.088	2183	2192	2221	rBV	199423	387099	91.71%	10.783%
16	8.850	2419	2429	2453	rBV	213688	354154	83.90%	9.865%
17	10.217	2842	2854	2868	rBV	60901	95493	22.62%	2.660%
18	11.246	3163	3174	3198	rBV	234322	359863	85.25%	10.024%
19	11.535	3255	3264	3277	rBV3	2325	4229	1.00%	0.118%
20	11.622	3280	3291	3314	rVB	185533	291027	68.95%	8.107%


Sum of corrected areas: 3590019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024627.D
Acq On : 12 Feb 2022 01:18
Operator : SY/MD
Sample : N1512-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

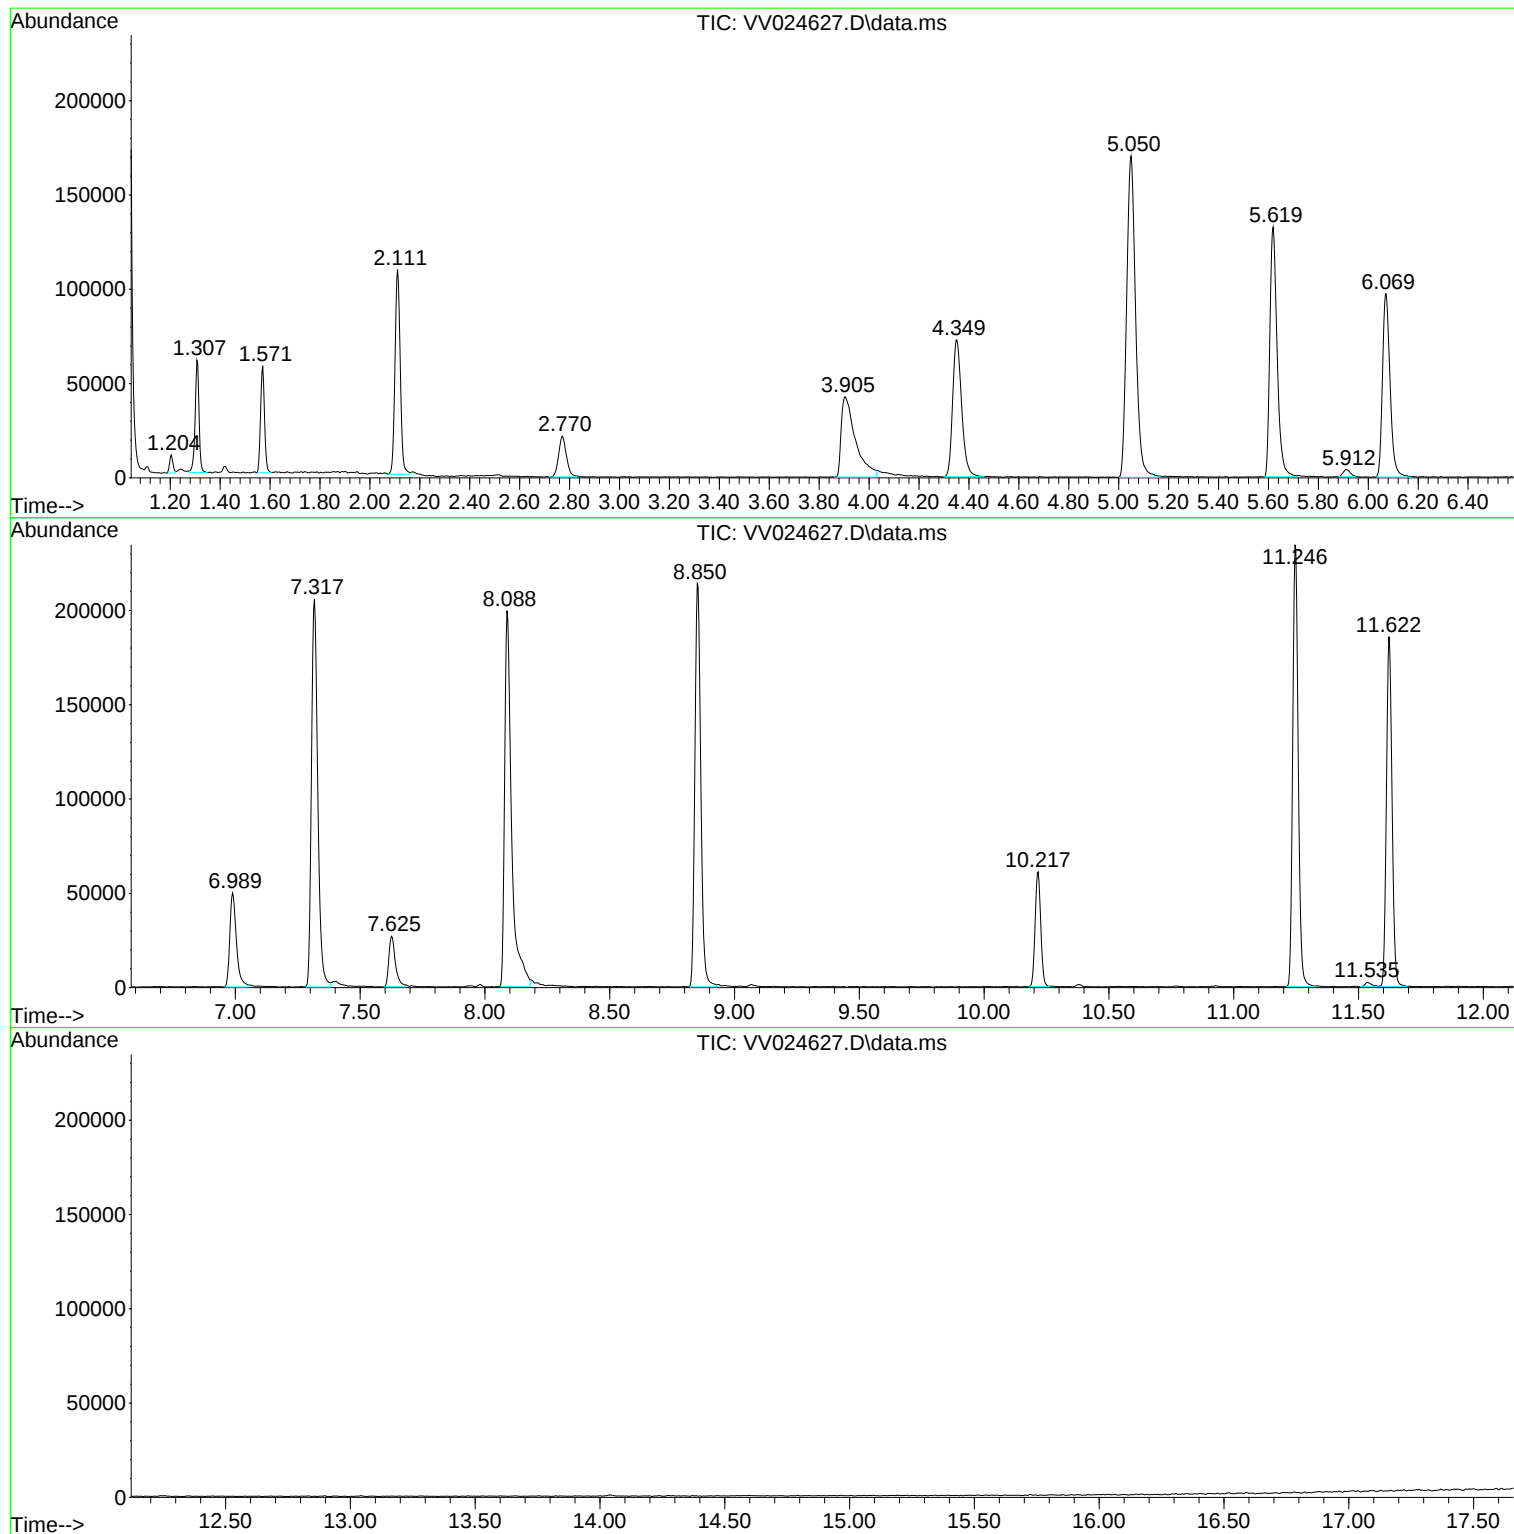

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024627.D
Acq On : 12 Feb 2022 01:18
Operator : SY/MD
Sample : N1512-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024627.D
Acq On : 12 Feb 2022 01:18
Operator : SY/MD
Sample : N1512-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc