

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024634.D
 Acq On : 12 Feb 2022 04:02
 Operator : SY/MD
 Sample : N1480-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCX1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	16	22	37	rVB	38442	37243	9.16%	1.049%
2	1.307	74	83	97	rBV2	63118	77557	19.08%	2.185%
3	1.420	110	118	124	rBV	7215	8547	2.10%	0.241%
4	1.571	157	165	175	rBV	54386	61365	15.10%	1.729%
5	2.111	323	333	348	rBV	102610	149209	36.71%	4.204%
6	3.896	875	888	930	rBV2	47454	160555	39.50%	4.524%
7	4.352	1013	1030	1058	rBV	71370	178683	43.96%	5.035%
8	5.050	1231	1247	1276	rBV2	162227	406469	100.00%	11.453%
9	5.619	1412	1424	1453	rBV	132312	269177	66.22%	7.584%
10	5.912	1507	1515	1533	rVB7	3650	8174	2.01%	0.230%
11	6.069	1551	1564	1595	rBV	92865	195260	48.04%	5.502%
12	6.989	1840	1850	1874	rBV2	44785	84500	20.79%	2.381%
13	7.317	1938	1952	1973	rBV	203030	351929	86.58%	9.916%
14	7.397	1973	1977	1995	rVB3	4031	7824	1.92%	0.220%
15	7.625	2039	2048	2068	rBV	25154	46401	11.42%	1.307%
16	8.088	2182	2192	2231	rBV	200112	381919	93.96%	10.761%
17	8.850	2418	2429	2453	rBV	216251	356405	87.68%	10.042%
18	10.214	2841	2853	2872	rBV2	59299	93692	23.05%	2.640%
19	11.246	3164	3174	3199	rBV	242561	368353	90.62%	10.379%
20	11.622	3279	3291	3307	rBV	181573	286173	70.40%	8.063%
21	16.310	4739	4749	4758	rBV2	13750	19616	4.83%	0.553%




Sum of corrected areas: 3549051

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024634.D
Acq On : 12 Feb 2022 04:02
Operator : SY/MD
Sample : N1480-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

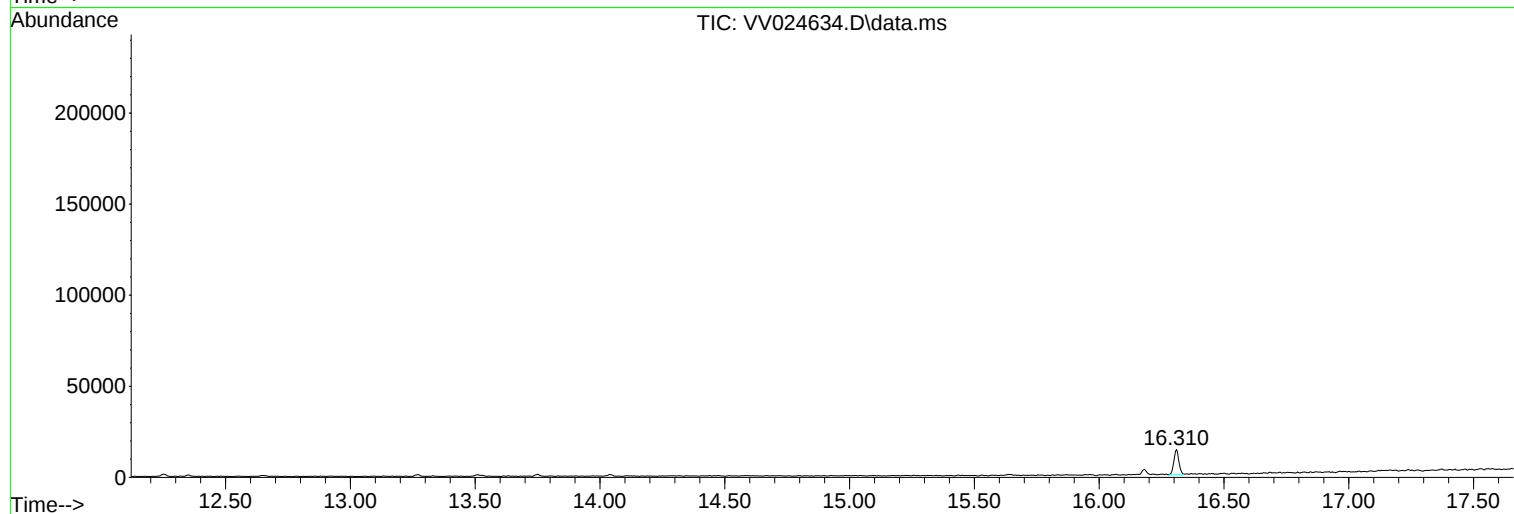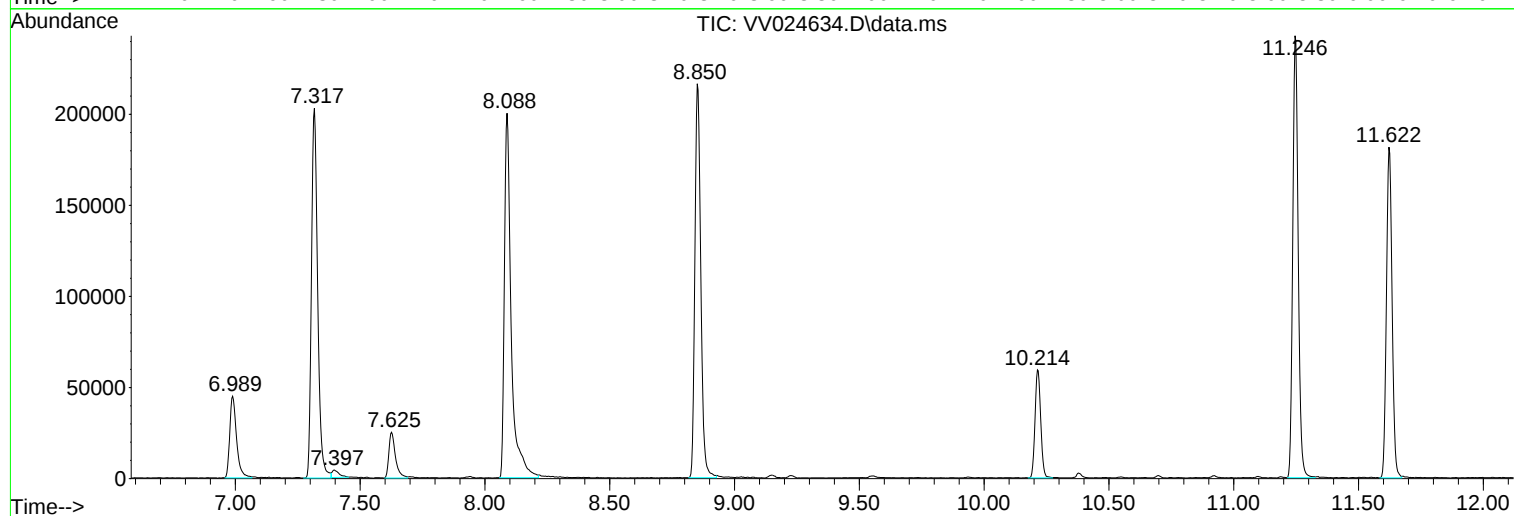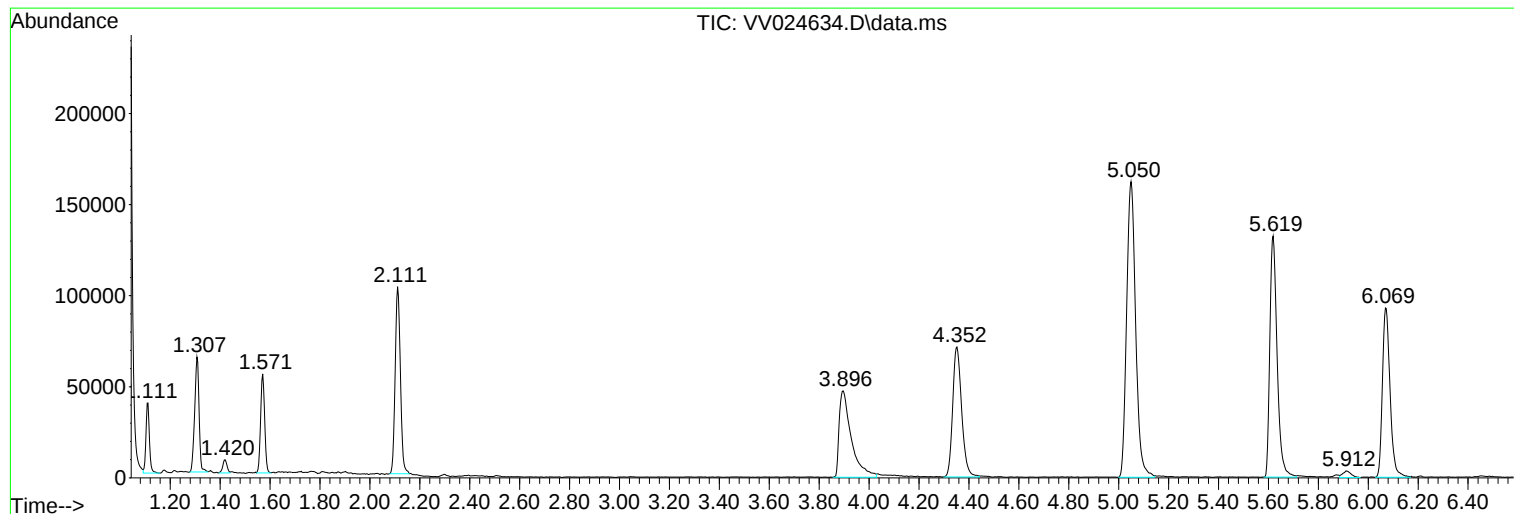

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024634.D
Acq On : 12 Feb 2022 04:02
Operator : SY/MD
Sample : N1480-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.111	0.69 ug/L	37243	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	86
2			Cyclopropane	42	C3H6	000075-19-4	64
3			Cyclopropane	42	C3H6	000075-19-4	64
4			Propene	42	C3H6	000115-07-1	38
5			Chloro(prop-2-yn-1-yloxy)methanone	118	C4H3ClO2	035718-08-2	23

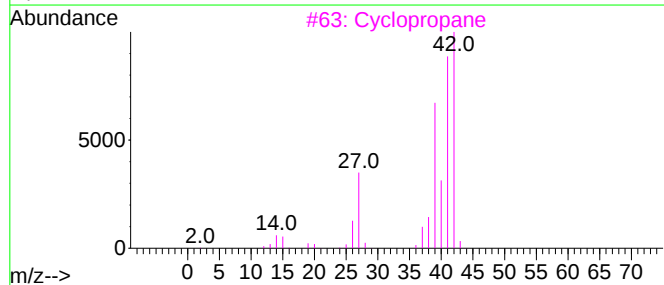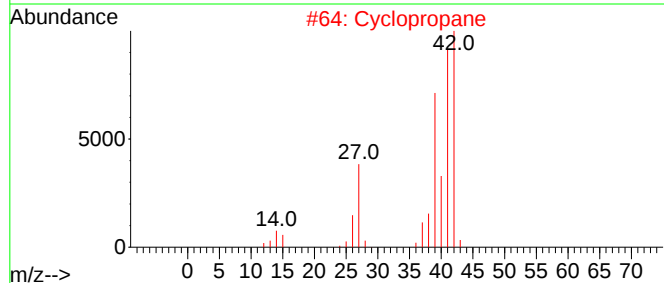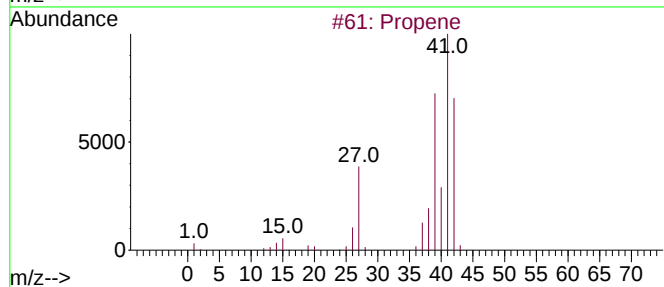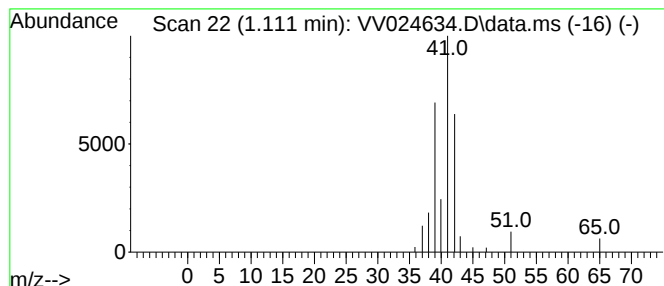

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024634.D
Acq On : 12 Feb 2022 04:02
Operator : SY/MD
Sample : N1480-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.111	0.7	ug/L	37243	1	5.619	269177	5.0