

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024636.D
 Acq On : 12 Feb 2022 04:48
 Operator : SY/MD
 Sample : N1480-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCX3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	97	rVB	58988	59466	14.56%	1.709%
2	1.571	157	165	175	rBV	54475	62213	15.23%	1.788%
3	2.111	323	333	352	rVB	106521	156657	38.36%	4.502%
4	3.474	754	757	765	rVB	9294	6194	1.52%	0.178%
5	3.895	879	888	915	rBV	41079	131433	32.18%	3.777%
6	4.352	1014	1030	1055	rBV2	71408	179755	44.02%	5.165%
7	5.050	1232	1247	1277	rBV2	165824	408392	100.00%	11.735%
8	5.619	1412	1424	1453	rBV2	129922	269330	65.95%	7.739%
9	5.908	1507	1514	1528	rBV5	2922	5707	1.40%	0.164%
10	6.072	1552	1565	1590	rBV	96483	198070	48.50%	5.692%
11	6.989	1834	1850	1873	rBV2	46297	88165	21.59%	2.533%
12	7.316	1940	1952	1973	rBV	202995	354496	86.80%	10.187%
13	7.403	1975	1979	1995	rVB2	2705	4688	1.15%	0.135%
14	7.625	2037	2048	2073	rBV2	26511	49343	12.08%	1.418%
15	8.088	2182	2192	2234	rBV	200978	381764	93.48%	10.970%
16	8.850	2418	2429	2454	rBV	214338	358261	87.72%	10.295%
17	10.217	2842	2854	2872	rVB	60006	95772	23.45%	2.752%
18	11.246	3164	3174	3195	rBV	235016	372639	91.25%	10.708%
19	11.622	3280	3291	3313	rBV	183390	291694	71.43%	8.382%
20	15.506	4492	4499	4506	rBB5	4436	6011	1.47%	0.173%




Sum of corrected areas: 3480050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024636.D
Acq On : 12 Feb 2022 04:48
Operator : SY/MD
Sample : N1480-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

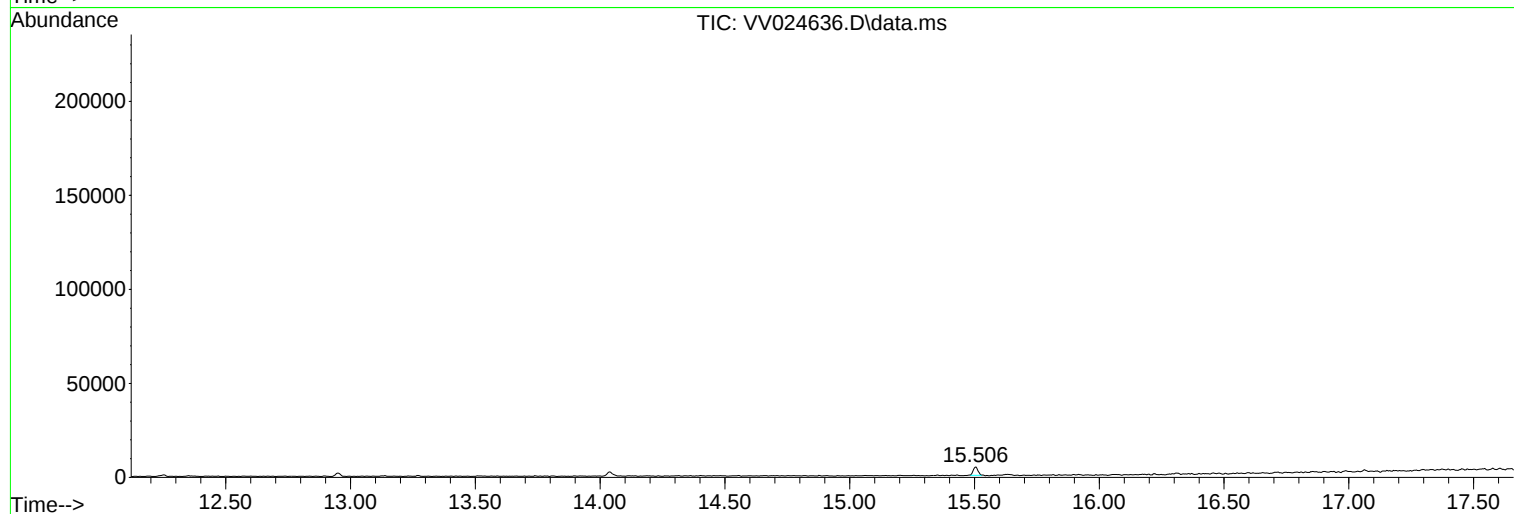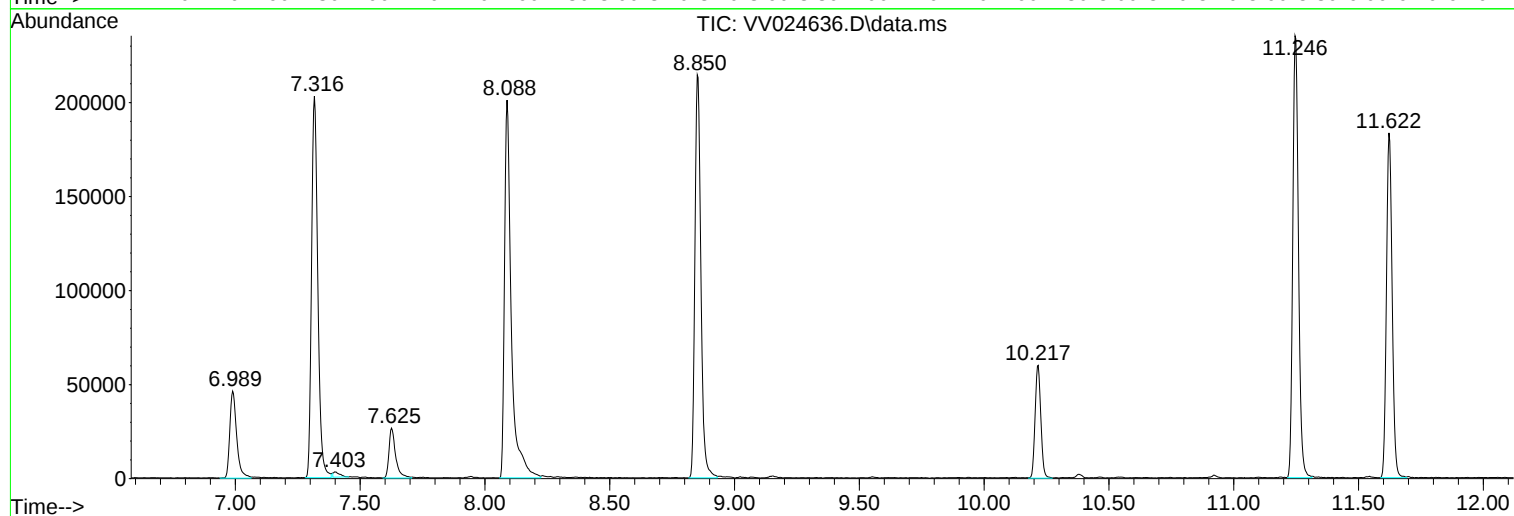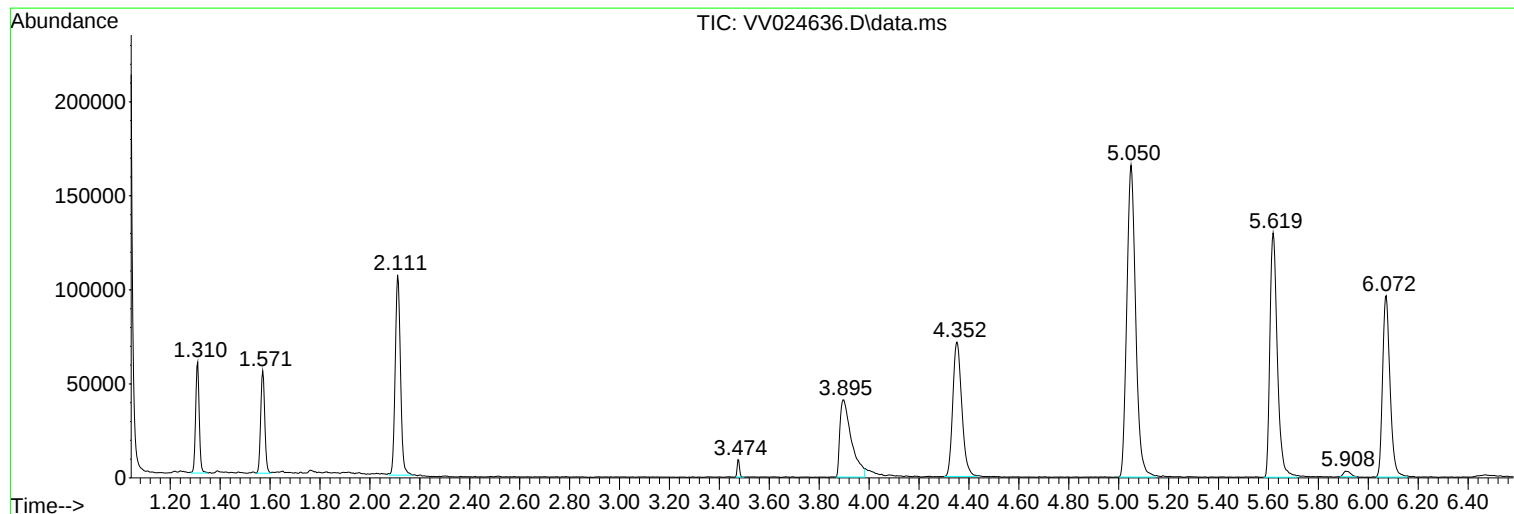

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024636.D
Acq On : 12 Feb 2022 04:48
Operator : SY/MD
Sample : N1480-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
Data File : VV024636.D
Acq On : 12 Feb 2022 04:48
Operator : SY/MD
Sample : N1480-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
