


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021122\
 Data File : VV024591.D
 Acq On : 11 Feb 2022 09:01
 Operator : SY/MD
 Sample : BFB268
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB268

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Feb 16 23:36:08 2022

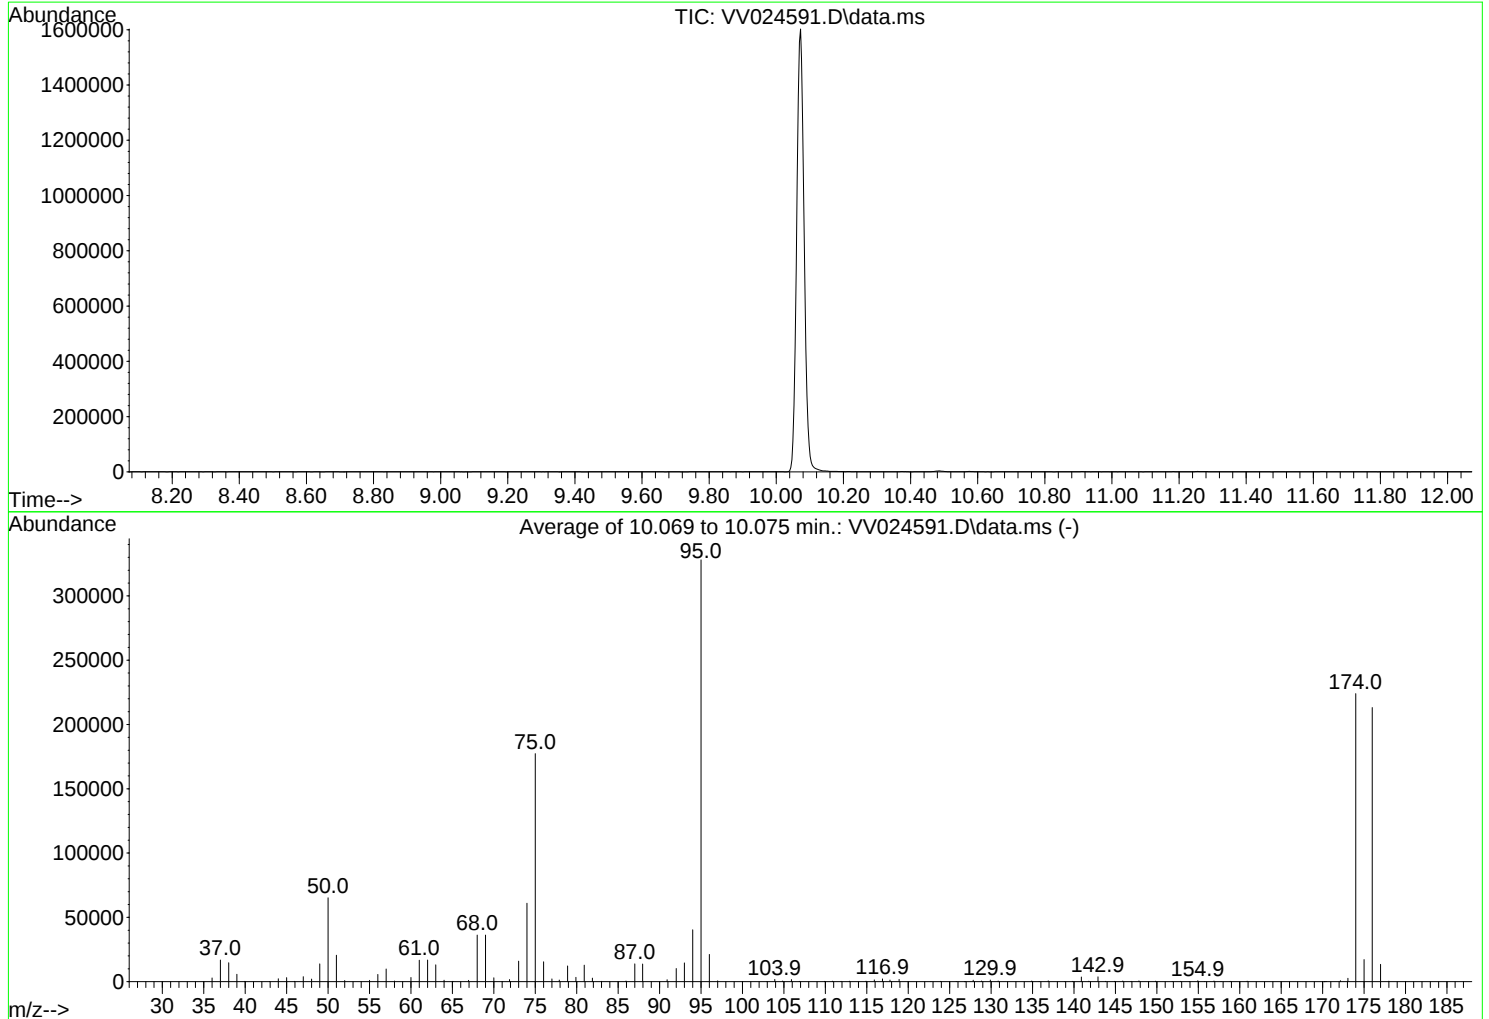

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	65192	PASS
75	95	30	80	54.0	177301	PASS
95	95	100	100	100.0	328064	PASS
96	95	5	9	6.5	21195	PASS
173	174	0.00	2	1.2	2588	PASS
174	95	50	120	68.3	224043	PASS
175	174	5	9	7.7	17244	PASS
176	174	95	105	95.2	213184	PASS
177	176	5	10	6.3	13462	PASS

m/z	Abundance
44.00	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
36.00	3032.0
37.00	17360.0
38.00	14954.0
39.00	5816.0
39.90	311.0
42.90	130.0
44.00	2572.0
45.00	3130.0
45.90	222.0
47.00	3965.0
48.00	2032.0
49.00	13979.0
50.00	67152.0
51.00	20864.0
52.00	875.0
55.00	1015.0
56.00	5811.0
57.00	10069.0
58.00	447.0
60.00	3420.0
61.00	16840.0
62.00	17280.0
63.00	13292.0
64.00	1110.0
65.00	304.0
66.90	1015.0
68.00	36864.0
69.00	36824.0
70.00	3002.0
71.00	120.0
71.90	1713.0
73.00	16327.0
74.00	61376.0
75.00	178624.0
76.00	15755.0
77.00	2164.0
77.90	1346.0
78.90	12313.0
79.90	3468.0
80.90	13069.0
81.90	2812.0
83.10	330.0
86.00	478.0
87.00	13853.0
87.90	13839.0
90.90	1542.0
92.00	10134.0
93.00	14788.0
94.00	40928.0
95.00	331840.0
96.00	21936.0
97.00	624.0
103.00	153.0
103.90	1678.0
104.80	449.0
105.90	1576.0
106.80	323.0
109.90	193.0
110.80	303.0
111.90	229.0
112.90	374.0
114.90	357.0
115.90	1461.0
116.90	2128.0
117.80	1223.0
118.90	1679.0
122.70	106.0
123.90	166.0
125.80	120.0
127.80	1093.0
128.90	560.0
129.90	1179.0
130.80	484.0
135.00	478.0
135.80	156.0
136.90	650.0
138.90	143.0
139.90	241.0
140.90	3444.0
141.80	420.0
142.90	3778.0
143.80	225.0
144.90	292.0
145.90	452.0
146.90	220.0
147.80	622.0
149.00	151.0
149.90	360.0
151.90	129.0
152.90	210.0
153.90	173.0
154.90	688.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

155.90	151.0
156.90	515.0
157.80	141.0
158.90	293.0
160.90	344.0
170.50	213.0
172.10	779.0
173.00	2535.0
174.00	219072.0
175.00	17480.0
176.00	207744.0
177.00	13497.0
178.00	429.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
36.00	3073.0
37.00	17400.0
38.00	15154.0
39.00	5892.0
40.00	320.0
42.90	156.0
44.00	2542.0
45.00	3163.0
46.00	233.0
47.00	3942.0
48.00	2047.0
49.00	14301.0
50.00	67304.0
51.00	21216.0
52.00	898.0
55.00	1008.0
56.00	5700.0
57.00	10024.0
58.00	506.0
60.00	3380.0
61.00	17272.0
62.00	17416.0
63.00	13541.0
64.00	1204.0
65.10	289.0
67.00	1028.0
68.00	37536.0
69.00	37424.0
70.00	3144.0
71.00	107.0
71.90	1665.0
73.00	16584.0
74.00	63224.0
75.00	183488.0
76.00	15886.0
77.00	2123.0
77.90	1332.0
78.90	12605.0
79.90	3511.0
80.90	13224.0
81.90	2823.0
83.00	300.0
86.00	514.0
87.00	14210.0
88.00	14111.0
90.90	1563.0
92.00	10520.0
93.00	14913.0
94.00	41592.0
95.00	339264.0
96.00	21896.0
97.00	597.0
103.00	160.0
103.90	1810.0
104.90	488.0
105.90	1713.0
106.80	287.0
109.90	201.0
110.80	351.0
111.90	221.0
112.90	403.0
114.90	366.0
115.90	1410.0
116.90	2121.0
117.80	1285.0
118.90	1765.0
122.70	126.0
123.90	203.0
125.80	127.0
126.80	102.0
127.80	1100.0
128.90	552.0
129.90	1242.0
130.90	463.0
134.90	516.0
135.80	161.0
136.90	675.0
138.90	107.0
139.80	234.0
140.90	3731.0
141.80	442.0
142.90	3877.0
143.80	229.0
144.90	258.0
145.90	483.0
146.90	220.0
147.90	657.0
149.00	194.0
149.90	343.0
151.80	151.0
152.90	231.0
153.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

155.00	776.0
155.80	132.0
156.90	594.0
157.80	146.0
158.90	287.0
160.90	346.0
170.40	191.0
172.10	769.0
173.00	2657.0
174.00	231616.0
175.00	17928.0
176.00	220544.0
177.00	13820.0
178.00	380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
36.00	2684.0
37.00	15786.0
38.00	14053.0
39.00	5419.0
40.00	305.0
43.00	155.0
44.00	2262.0
45.00	2944.0
46.00	240.0
47.00	3629.0
48.00	1937.0
49.00	13347.0
50.00	61120.0
51.00	19528.0
52.00	830.0
55.00	952.0
56.00	5159.0
57.00	9316.0
58.00	482.0
60.00	3009.0
61.00	15871.0
62.00	15694.0
63.00	12298.0
64.00	1108.0
65.10	249.0
67.00	921.0
68.00	34320.0
69.00	34320.0
70.00	2902.0
71.00	106.0
71.90	1596.0
73.00	14970.0
74.00	58280.0
75.00	169792.0
76.00	14638.0
77.00	1986.0
77.90	1161.0
78.90	11653.0
79.90	3213.0
80.90	12228.0
81.90	2484.0
82.90	292.0
85.90	466.0
87.00	13242.0
88.00	12991.0
90.90	1440.0
92.00	10102.0
93.00	13887.0
94.00	38584.0
95.00	313088.0
96.00	19752.0
97.00	548.0
102.90	161.0
103.90	1699.0
104.90	492.0
105.90	1702.0
106.90	265.0
109.90	192.0
110.90	407.0
111.90	219.0
112.90	353.0
114.90	341.0
115.90	1230.0
116.90	1985.0
117.80	1275.0
118.90	1734.0
122.80	105.0
123.90	216.0
125.80	114.0
126.80	125.0
127.90	1036.0
128.80	497.0
129.90	1185.0
130.90	404.0
134.80	538.0
135.80	155.0
136.90	606.0
139.80	214.0
140.90	3597.0
141.80	404.0
142.90	3638.0
143.80	206.0
144.90	204.0
145.90	428.0
146.90	213.0
147.90	686.0
149.00	201.0
149.70	307.0
151.80	168.0
152.80	216.0
153.90	166.0
154.90	765.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

155.70	110.0
156.90	606.0
157.70	118.0
158.80	268.0
160.90	320.0
170.20	175.0
172.20	678.0
173.10	2572.0
174.00	221440.0
175.00	16324.0
176.00	211264.0
177.00	13070.0
178.00	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268