




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034149.D
Acq On : 13 Feb 2024 12:48
Operator : SY/MD
Sample : P1402-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

Quant Time: Feb 14 01:42:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

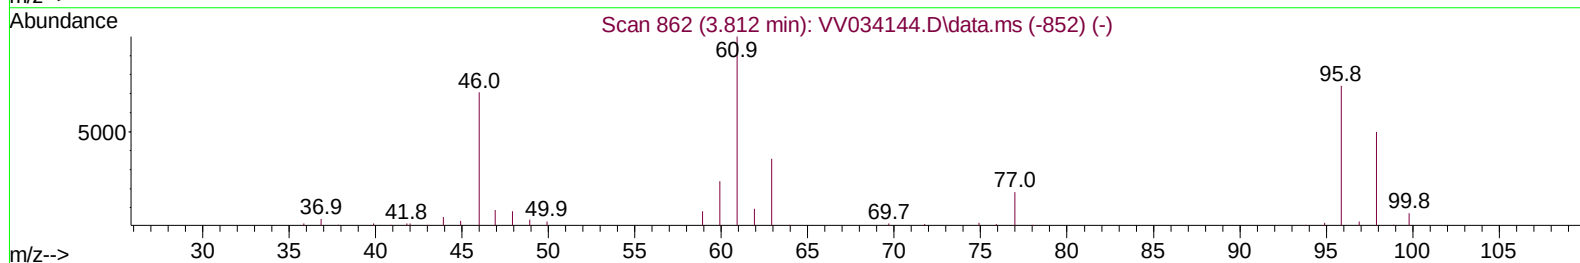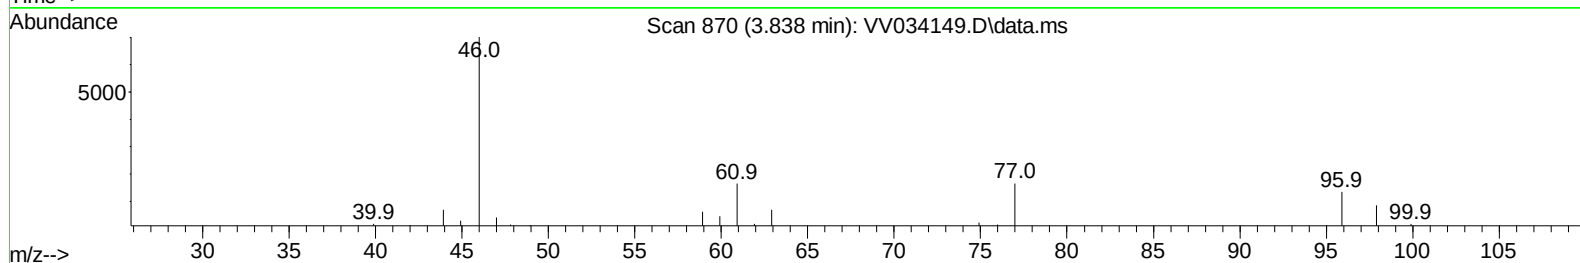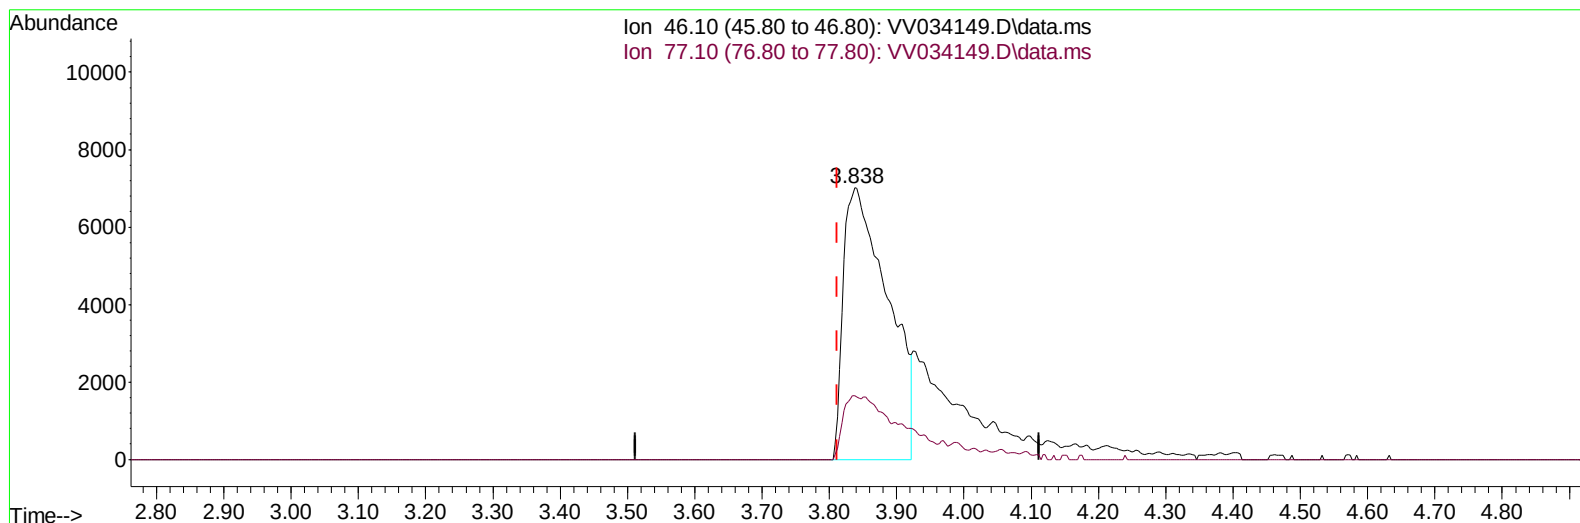

TIC: VV034149.D\data.ms

(20) 2-Butanone-d5 (S)**3.838min (+ 0.026) 30.66 ug/L****response 32142**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	9.45#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034149.D
Acq On : 13 Feb 2024 12:48
Operator : SY/MD
Sample : P1402-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

Quant Time: Feb 14 01:42:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

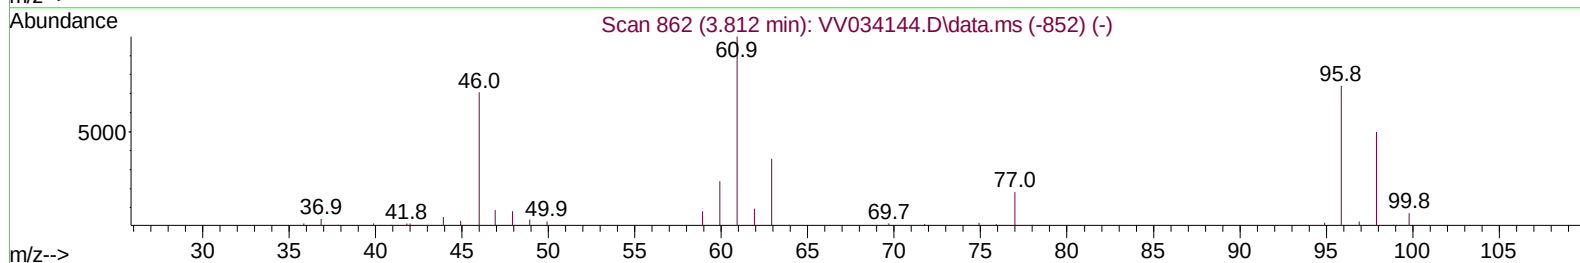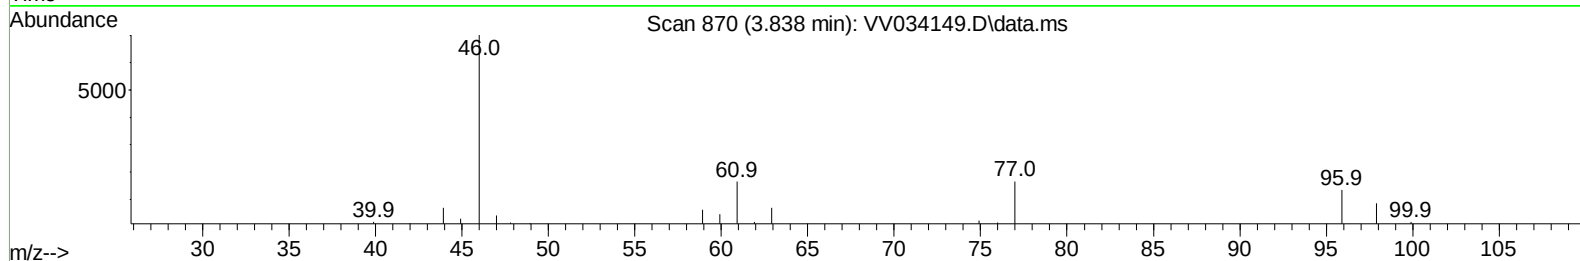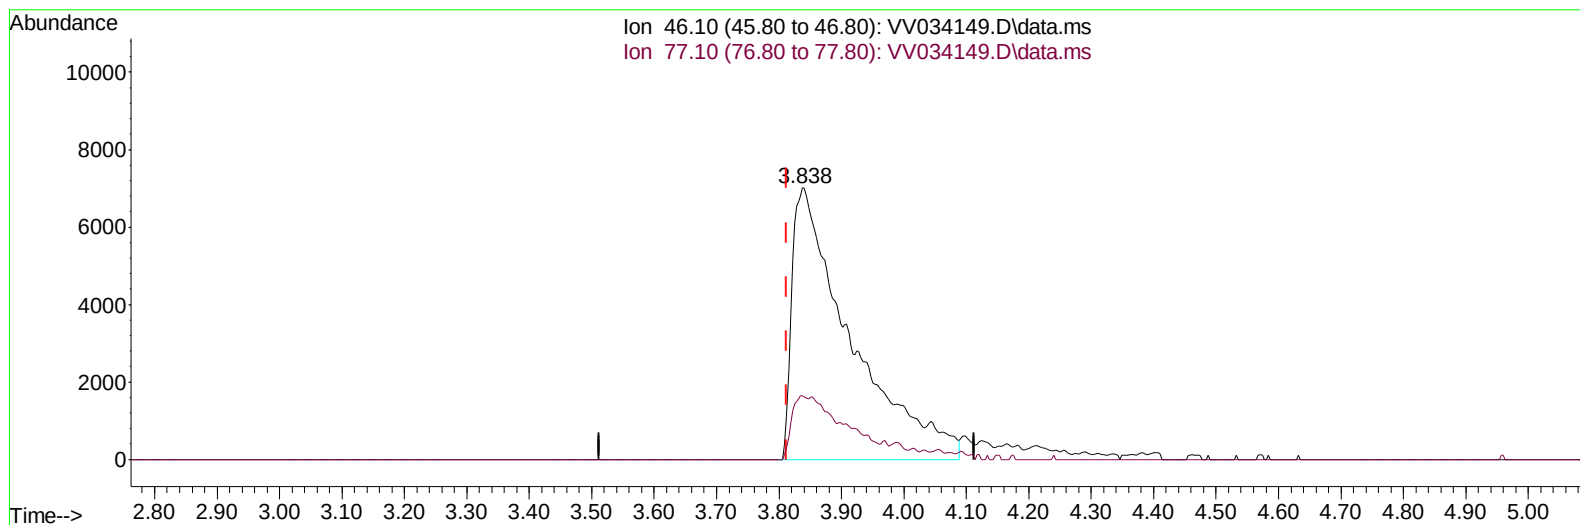

TIC: VV034149.D\data.ms

(20) 2-Butanone-d5 (S)**3.838min (+ 0.026) 43.54 ug/L m****response 45644**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	6.66#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034149.D
 Acq On : 13 Feb 2024 12:48
 Operator : SY/MD
 Sample : P1402-10DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE0DL

Manual IntegrationsAPPROVED

Quant Time: Feb 14 01:42:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 14 01:41:00 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 02/14/2024
 Supervised By :Semsettin Yesilyurt 02/14/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	80592	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	74070	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	34993	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	26139	4.188	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	83.800%		
7) Chloroethane-d5	1.532	69	23478	4.294	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	85.800%		
11) 1,1-Dichloroethene-d2	2.060	65	12522	4.160	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	83.200%		
20) 2-Butanone-d5	3.838	46	45644m	43.542	ug/L	0.03
Spiked Amount 50.000	Range 40 - 130		Recovery =	87.080%		
24) Chloroform-d	4.249	84	50905	4.488	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.800%		
26) 1,2-Dichloroethane-d4	4.947	65	25620	4.834	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	96.600%		
32) Benzene-d6	4.960	84	96966	4.363	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	87.200%		
36) 1,2-Dichloropropane-d6	5.989	67	27559	4.436	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	88.800%		
41) Toluene-d8	7.243	98	86043	4.213	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	84.200%		
43) trans-1,3-Dichloroprop...	7.561	79	10521	4.485	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	89.800%		
46) 2-Hexanone-d5	8.030	63	32643	38.984	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	77.960%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	15742	4.180	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	83.600%		
66) 1,2-Dichlorobenzene-d4	11.561	152	29761	4.676	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	93.600%		
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.069	96	2022	0.359	ug/L #	1
22) cis-1,2-Dichloroethene	3.822	96	5357	0.823	ug/L	88
34) Trichloroethene	5.831	95	43140	6.710	ug/L	98
47) Tetrachloroethene	7.905	164	5894	1.128	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034149.D
Acq On : 13 Feb 2024 12:48
Operator : SY/MD
Sample : P1402-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE0DL

Manual IntegrationsAPPROVED

Quant Time: Feb 14 01:42:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

