




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

Quant Time: Feb 14 01:45:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

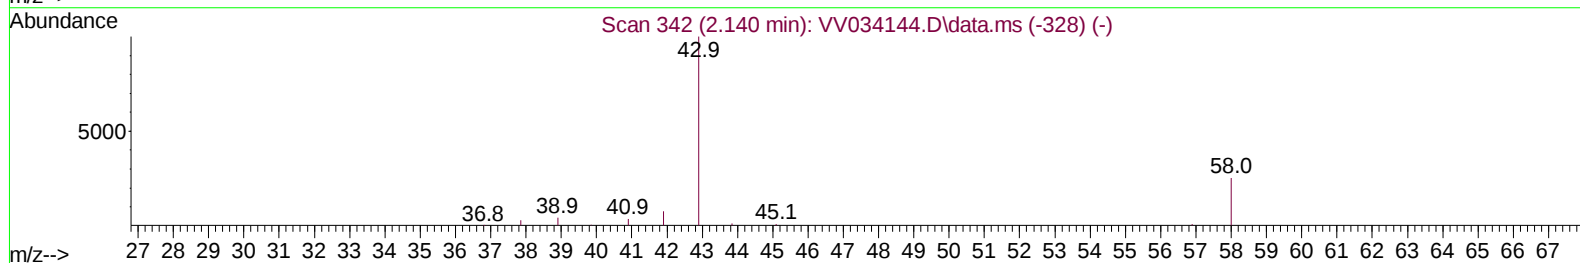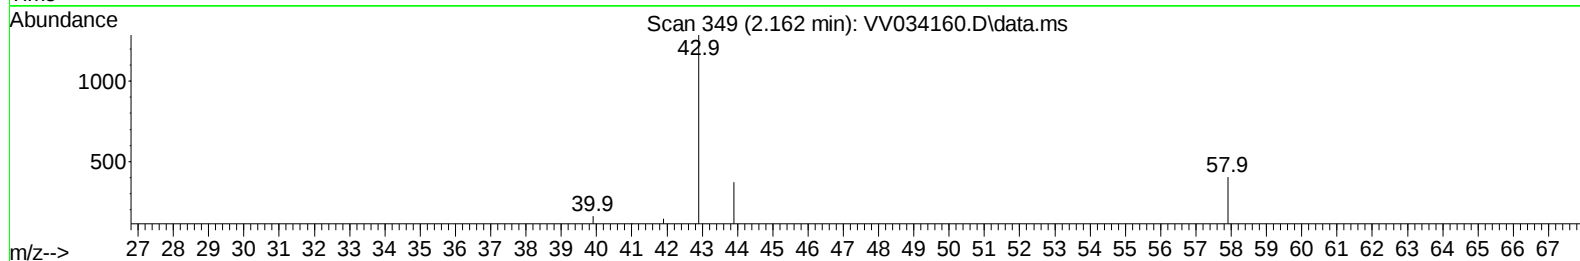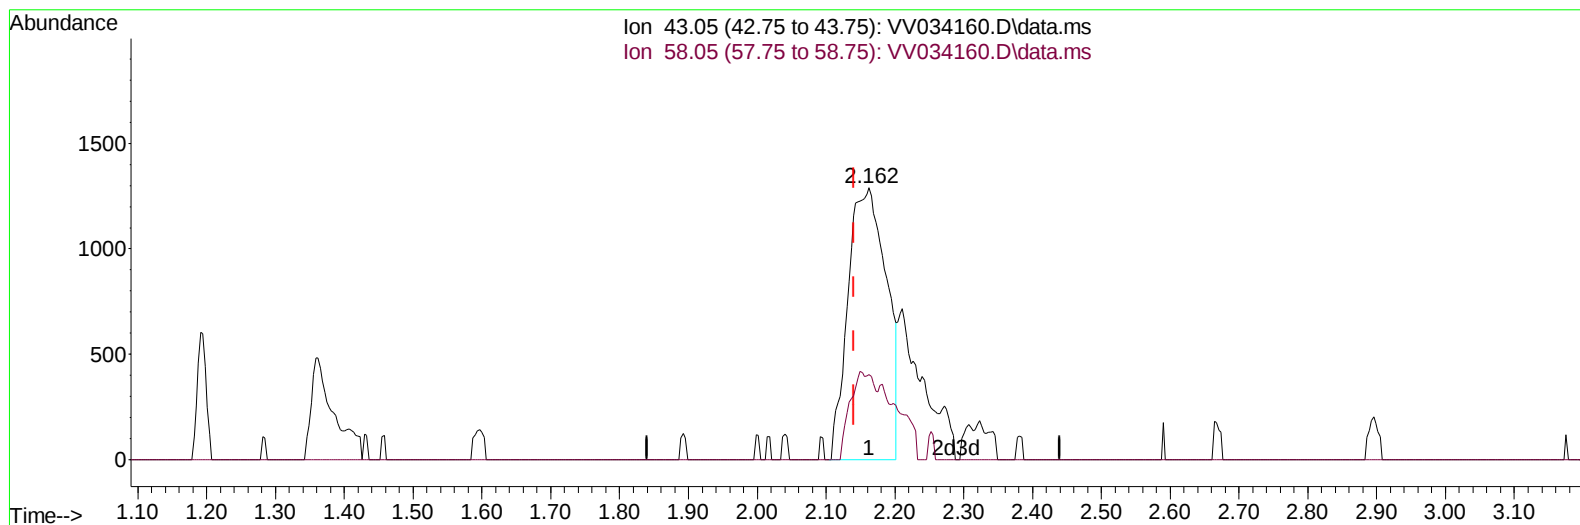

TIC: VV034160.D\data.ms

(13) Acetone (T)

2.162min (+ 0.022) 6.49 ug/L

response 4956

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	21.43#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

Quant Time: Feb 14 01:45:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

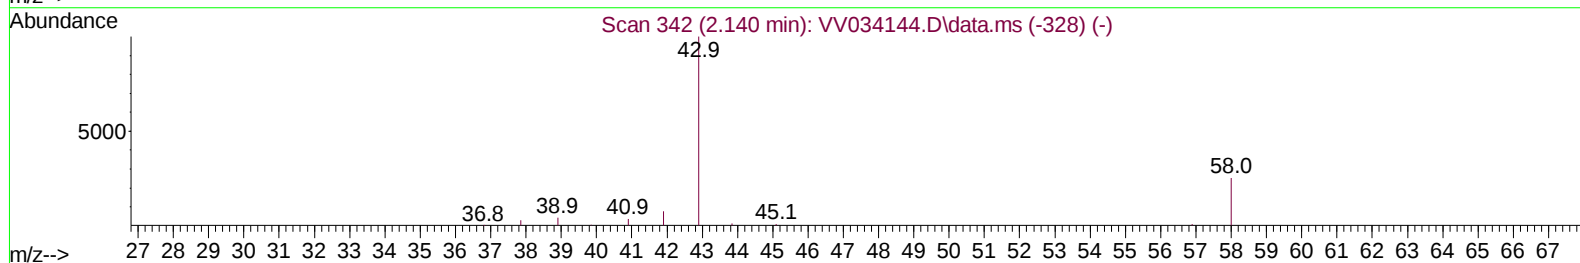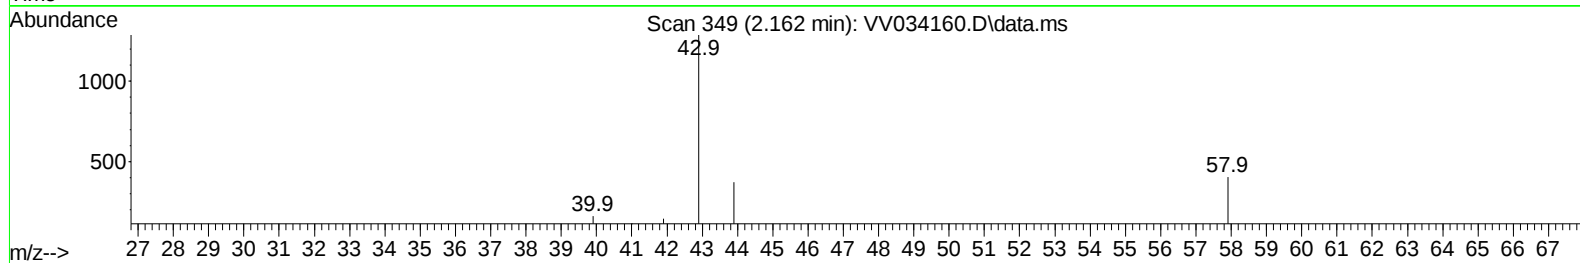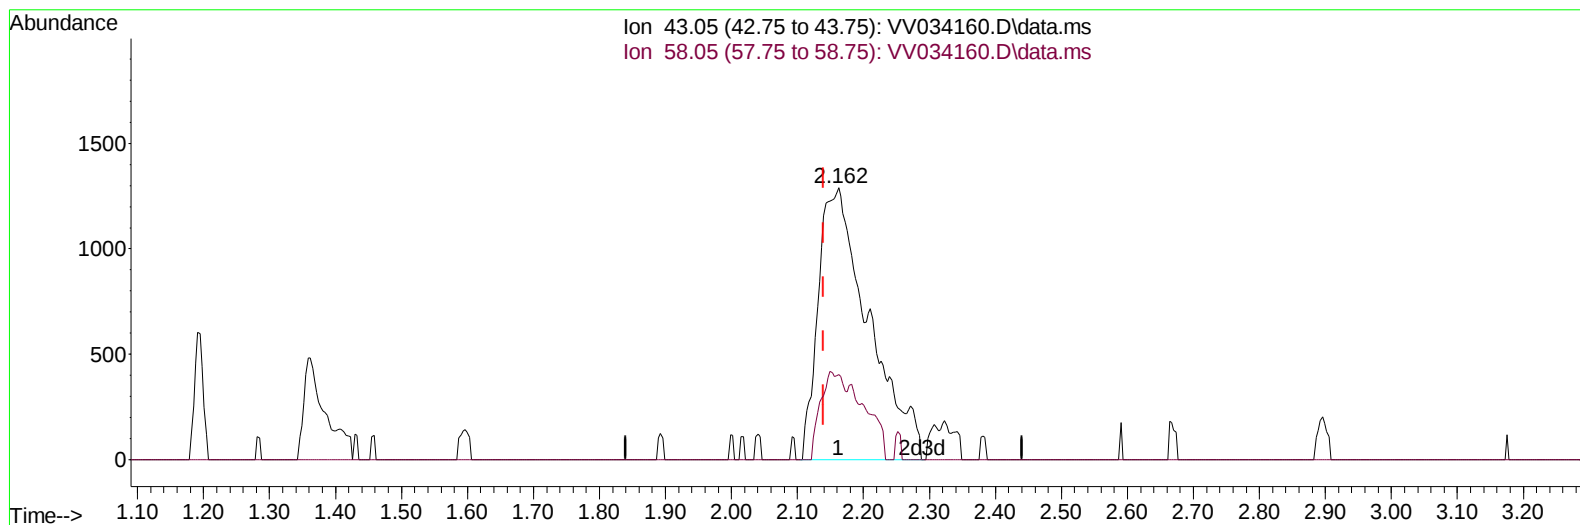

TIC: VV034160.D\data.ms

(13) Acetone (T)

2.162min (+ 0.022) 8.92 ug/L m

response 6810

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	6.90	15.59#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034160.D
 Acq On : 13 Feb 2024 18:20
 Operator : SY/MD
 Sample : P1402-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Manual IntegrationsAPPROVED

Quant Time: Feb 14 01:45:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 14 01:41:00 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 02/14/2024
 Supervised By :Semsettin Yesilyurt 02/14/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		77382	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		72727	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152		37751	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		22643	3.778	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	75.600%		
7) Chloroethane-d5	1.535	69		20795	3.961	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	79.200%		
11) 1,1-Dichloroethene-d2	2.060	65		11292	3.907	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	78.200%		
20) 2-Butanone-d5	3.828	46		36388	36.152	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery =	72.300%		
24) Chloroform-d	4.252	84		46464	4.267	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	85.400%		
26) 1,2-Dichloroethane-d4	4.947	65		24033	4.722	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	94.400%		
32) Benzene-d6	4.963	84		86452	3.962	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	79.200%		
36) 1,2-Dichloropropane-d6	5.992	67		24214	3.970	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	79.400%		
41) Toluene-d8	7.246	98		80759	4.027	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	80.600%		
43) trans-1,3-Dichloroprop...	7.561	79		9137	3.967	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	79.400%		
46) 2-Hexanone-d5	8.030	63		30482	37.075	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	74.160%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84		15212	4.114	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	82.200%		
66) 1,2-Dichlorobenzene-d4	11.561	152		29813	4.342	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	86.800%		
Target Compounds							
13) Acetone	2.162	43		6810m	8.918	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Manual IntegrationsAPPROVED

Quant Time: Feb 14 01:45:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 14 01:41:00 2024
Response via : Initial Calibration

Reviewed By :John Carlone 02/14/2024
Supervised By :Semsettin Yesilyurt 02/14/2024

