

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034147.D
 Acq On : 13 Feb 2024 10:57
 Operator : SY/MD
 Sample : P1402-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	91	rVB	36323	41924	16.90%	1.995%
2	1.536	146	154	165	rVB	34133	39030	15.74%	1.857%
3	2.063	307	318	331	rBV	68834	100821	40.65%	4.797%
4	2.130	331	339	354	rVB4	1964	4649	1.87%	0.221%
5	2.372	402	414	430	rBV4	3929	12316	4.97%	0.586%
6	2.449	430	438	450	rVV	10946	18979	7.65%	0.903%
7	2.516	453	459	471	rVB2	2100	3254	1.31%	0.155%
8	3.806	852	860	895	rBV2	20059	66145	26.67%	3.147%
9	4.253	984	999	1025	rBV2	45191	129748	52.31%	6.173%
10	4.960	1203	1219	1246	rBV2	99433	248029	100.00%	11.801%
11	5.535	1387	1398	1424	rBV	85162	175649	70.82%	8.357%
12	5.989	1528	1539	1562	rBV2	53486	111273	44.86%	5.294%
13	6.918	1818	1828	1847	rBV	25363	49249	19.86%	2.343%
14	7.243	1919	1929	1951	rBV	121563	219105	88.34%	10.425%
15	7.558	2020	2027	2047	rBV	13788	25615	10.33%	1.219%
16	8.027	2165	2173	2210	rBV	87309	188883	76.15%	8.987%
17	8.786	2399	2409	2430	rBV	128140	217247	87.59%	10.336%
18	10.153	2825	2834	2847	rBV2	33326	51961	20.95%	2.472%
19	11.185	3145	3155	3179	rBV	139813	215797	87.00%	10.267%
20	11.561	3262	3272	3291	rBV	114906	182121	73.43%	8.665%




Sum of corrected areas: 2101795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034147.D
Acq On : 13 Feb 2024 10:57
Operator : SY/MD
Sample : P1402-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

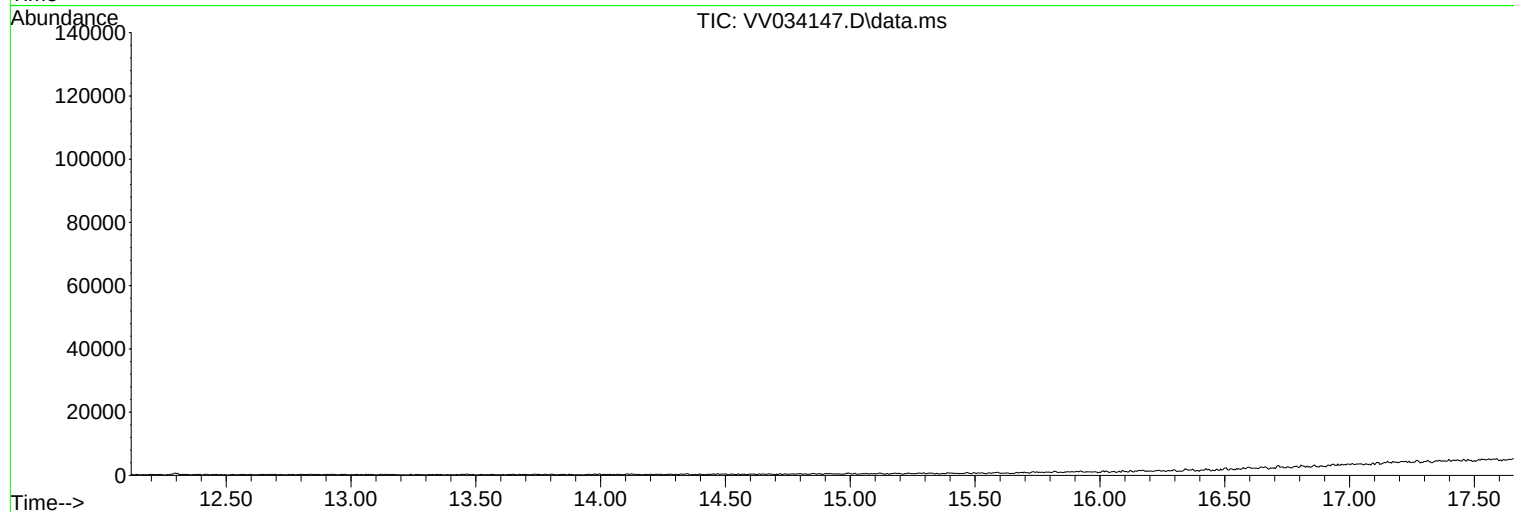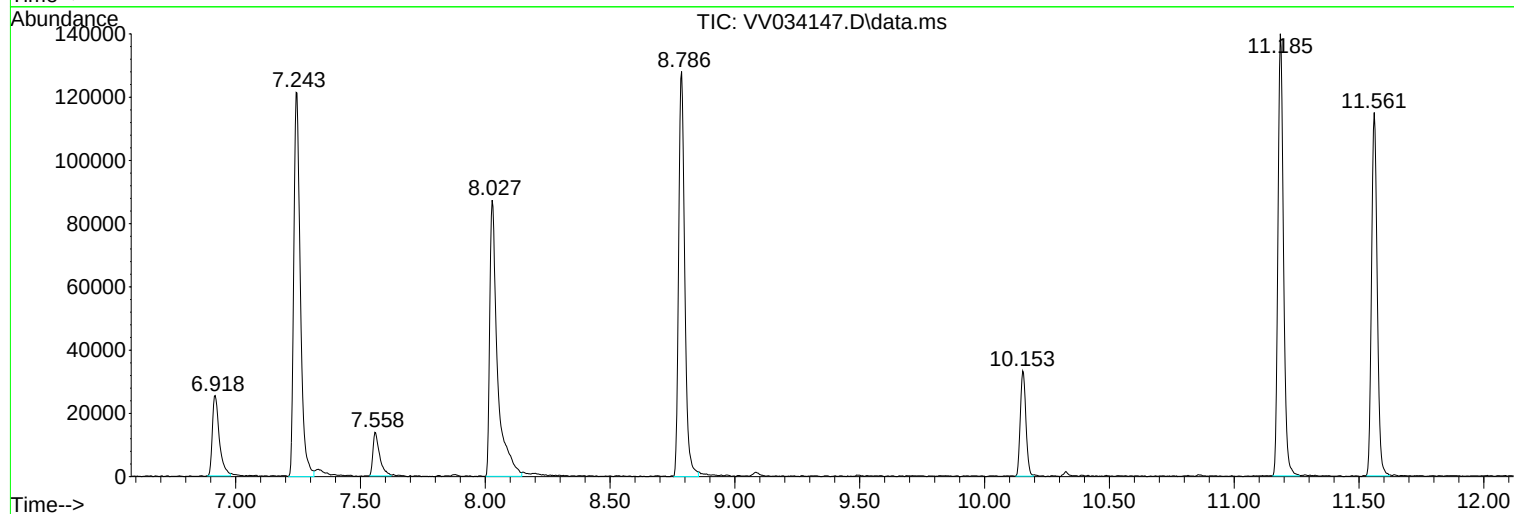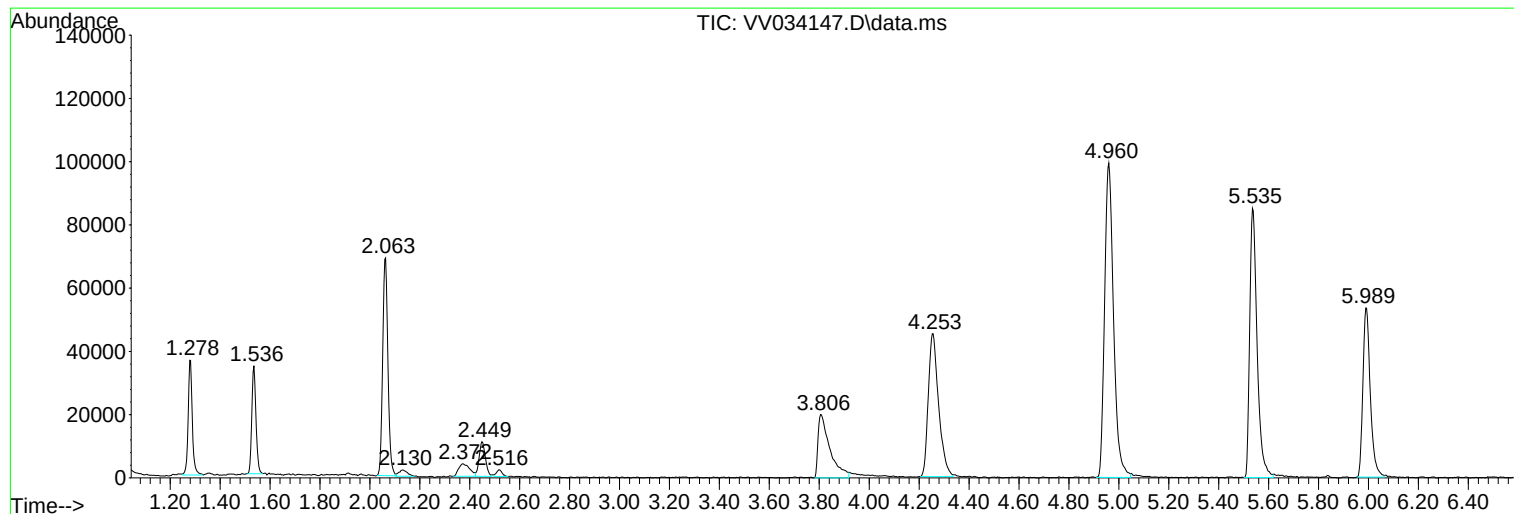

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034147.D
Acq On : 13 Feb 2024 10:57
Operator : SY/MD
Sample : P1402-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034147.D
Acq On : 13 Feb 2024 10:57
Operator : SY/MD
Sample : P1402-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc