

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034148.D
 Acq On : 13 Feb 2024 11:21
 Operator : SY/MD
 Sample : P1402-07DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	34122	37083	15.99%	1.654%
2	1.535	145	154	165	rVB	32805	38511	16.60%	1.717%
3	2.060	304	317	335	rBV	66121	99480	42.88%	4.436%
4	2.452	429	439	451	rVB4	4208	7176	3.09%	0.320%
5	3.818	853	864	897	rBV3	36114	108589	46.81%	4.842%
6	4.252	983	999	1031	rBV3	39776	104955	45.24%	4.680%
7	4.960	1205	1219	1246	rBV2	93433	231973	100.00%	10.344%
8	5.535	1387	1398	1419	rBV	83727	173149	74.64%	7.721%
9	5.834	1480	1491	1516	rBV2	89255	180912	77.99%	8.067%
10	5.992	1528	1540	1565	rBV	50275	104858	45.20%	4.676%
11	6.918	1812	1828	1855	rBV2	23870	48979	21.11%	2.184%
12	7.246	1919	1930	1961	rBV	111502	203546	87.75%	9.076%
13	7.561	2019	2028	2045	rBV2	12755	24287	10.47%	1.083%
14	7.908	2127	2136	2152	rVB	25608	43816	18.89%	1.954%
15	8.027	2165	2173	2210	rBV	80705	176538	76.10%	7.872%
16	8.786	2399	2409	2435	rBV	125721	214045	92.27%	9.544%
17	10.156	2825	2835	2852	rVB2	30839	49813	21.47%	2.221%
18	10.326	2880	2888	2898	rVB3	1554	2430	1.05%	0.108%
19	11.185	3143	3155	3185	rVB	138100	216508	93.33%	9.654%
20	11.561	3261	3272	3293	rBV	110329	175962	75.85%	7.846%




Sum of corrected areas: 2242610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034148.D
Acq On : 13 Feb 2024 11:21
Operator : SY/MD
Sample : P1402-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

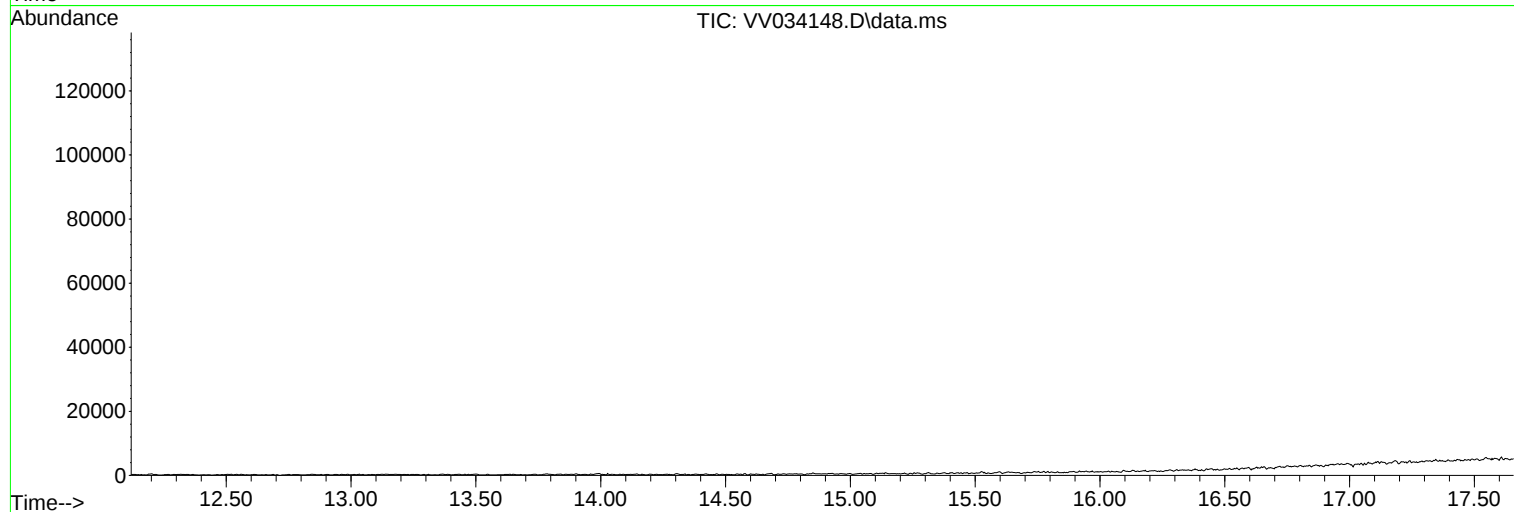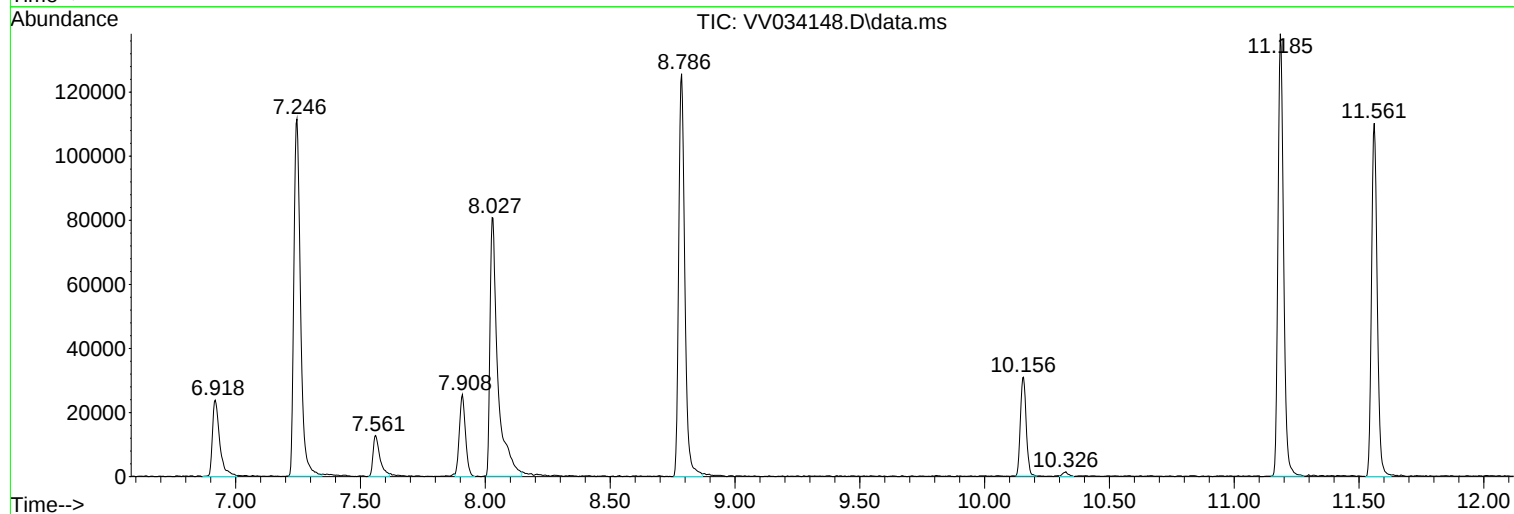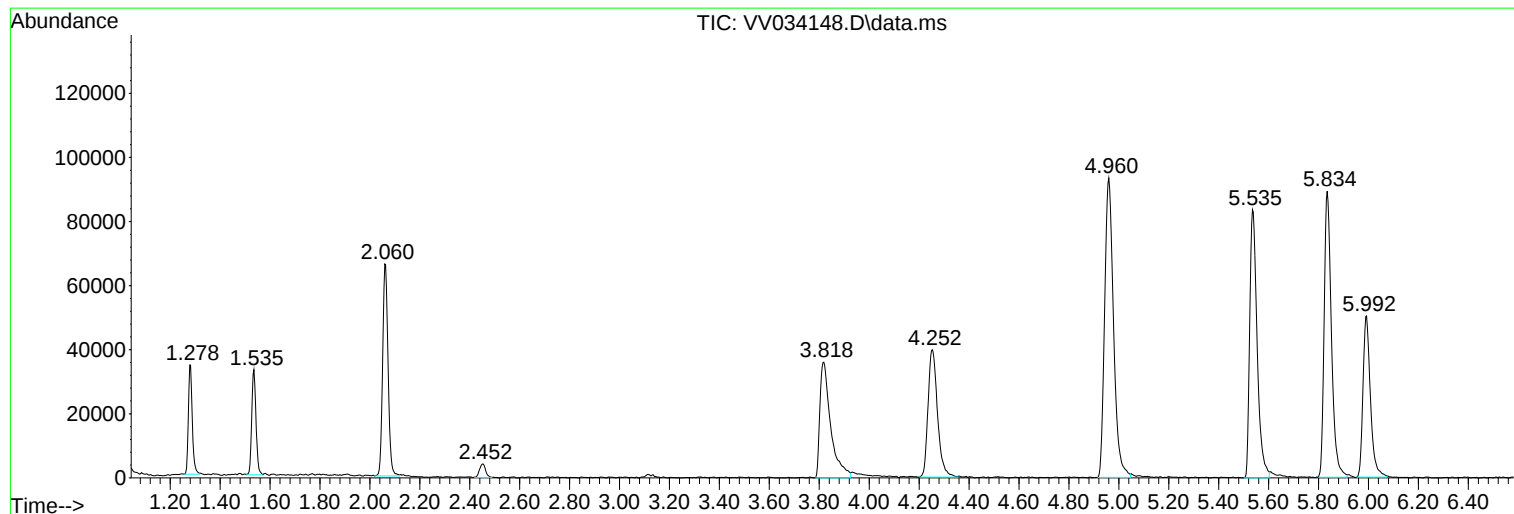

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034148.D
Acq On : 13 Feb 2024 11:21
Operator : SY/MD
Sample : P1402-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034148.D
Acq On : 13 Feb 2024 11:21
Operator : SY/MD
Sample : P1402-07DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc