

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034151.D
 Acq On : 13 Feb 2024 13:35
 Operator : SY/MD
 Sample : P1402-13DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	63	74	87	rBV	36230	39761	15.36%	1.402%
2	1.536	146	154	167	rVB	35152	42121	16.28%	1.485%
3	2.066	308	319	341	rVB3	123758	211232	81.62%	7.447%
4	2.449	432	438	447	rBV3	2155	3611	1.40%	0.127%
5	3.117	633	646	668	rVB2	9035	19211	7.42%	0.677%
6	3.818	852	864	896	rBV2	57527	167215	64.62%	5.895%
7	4.252	984	999	1026	rBV2	44396	117890	45.56%	4.156%
8	4.519	1067	1082	1093	rBV5	3477	8287	3.20%	0.292%
9	4.960	1205	1219	1251	rBV3	102907	258784	100.00%	9.124%
10	5.535	1388	1398	1430	rBV	90506	187014	72.27%	6.593%
11	5.834	1480	1491	1519	rBV	114232	232189	89.72%	8.186%
12	5.989	1528	1539	1563	rBV2	54959	114306	44.17%	4.030%
13	6.918	1817	1828	1856	rBV	27362	54531	21.07%	1.923%
14	7.243	1918	1929	1956	rBV	129293	229981	88.87%	8.108%
15	7.561	2019	2028	2053	rBV2	14593	29485	11.39%	1.040%
16	7.905	2124	2135	2153	rBV	131863	221231	85.49%	7.800%
17	8.027	2164	2173	2212	rBV	93799	200851	77.61%	7.081%
18	8.786	2398	2409	2434	rBV	132838	224811	86.87%	7.926%
19	10.153	2823	2834	2845	rBV2	35576	56332	21.77%	1.986%
20	11.185	3145	3155	3181	rBV	142936	224301	86.67%	7.908%
21	11.561	3258	3272	3296	rBV	119713	193270	74.68%	6.814%




Sum of corrected areas: 2836414

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034151.D
Acq On : 13 Feb 2024 13:35
Operator : SY/MD
Sample : P1402-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

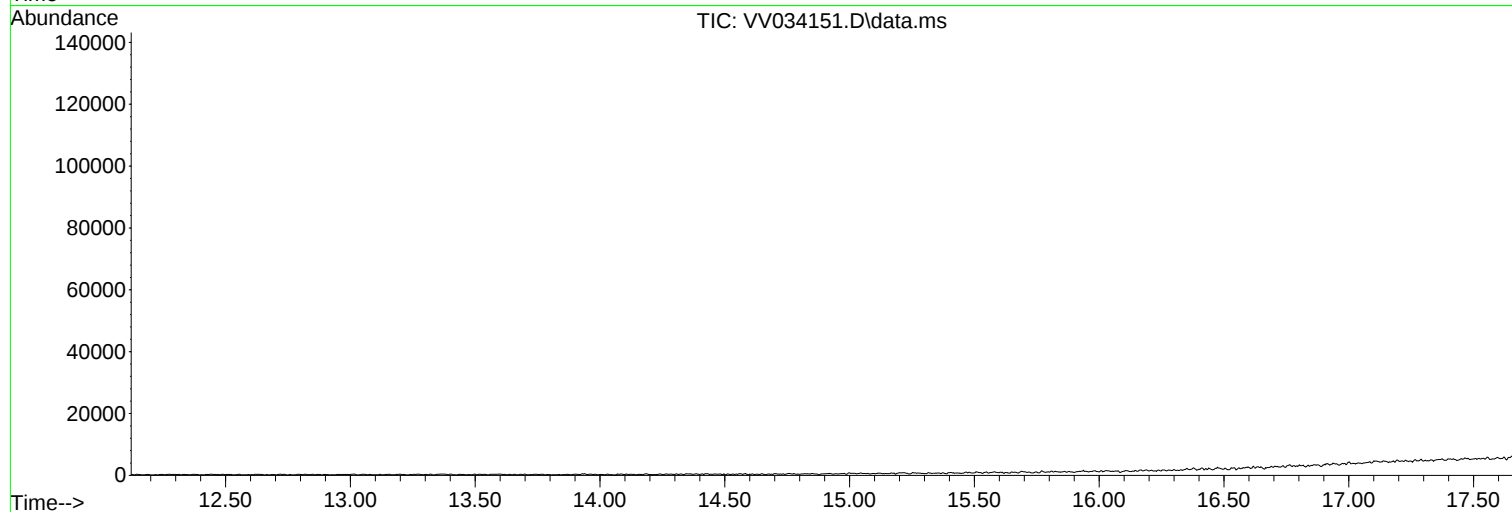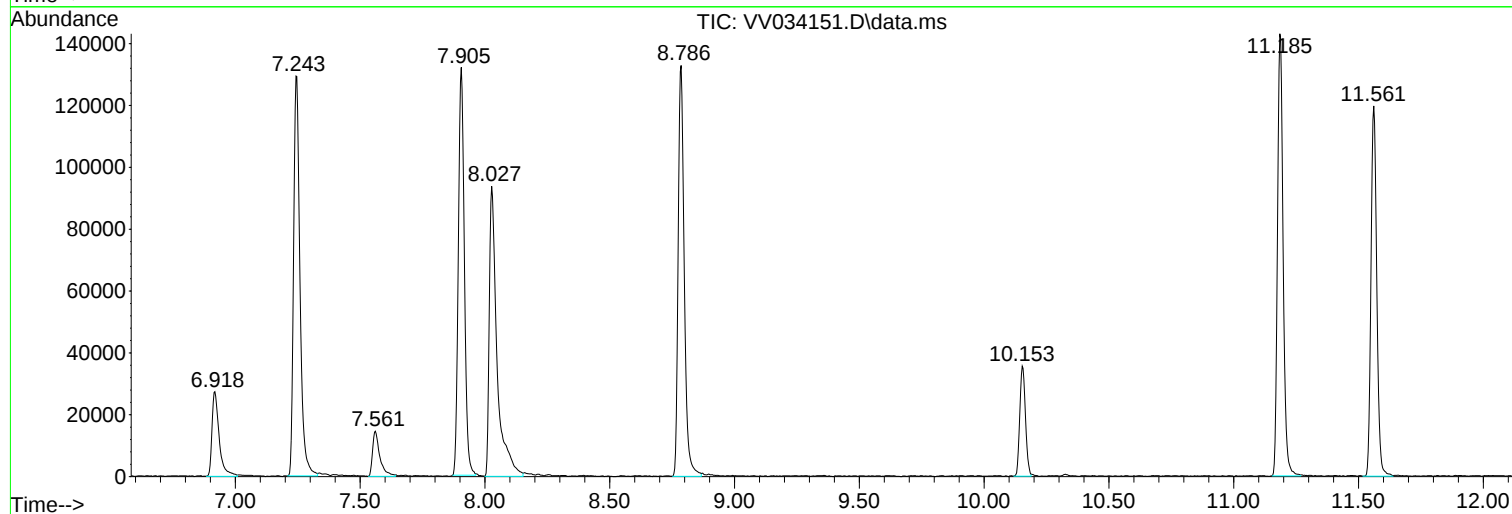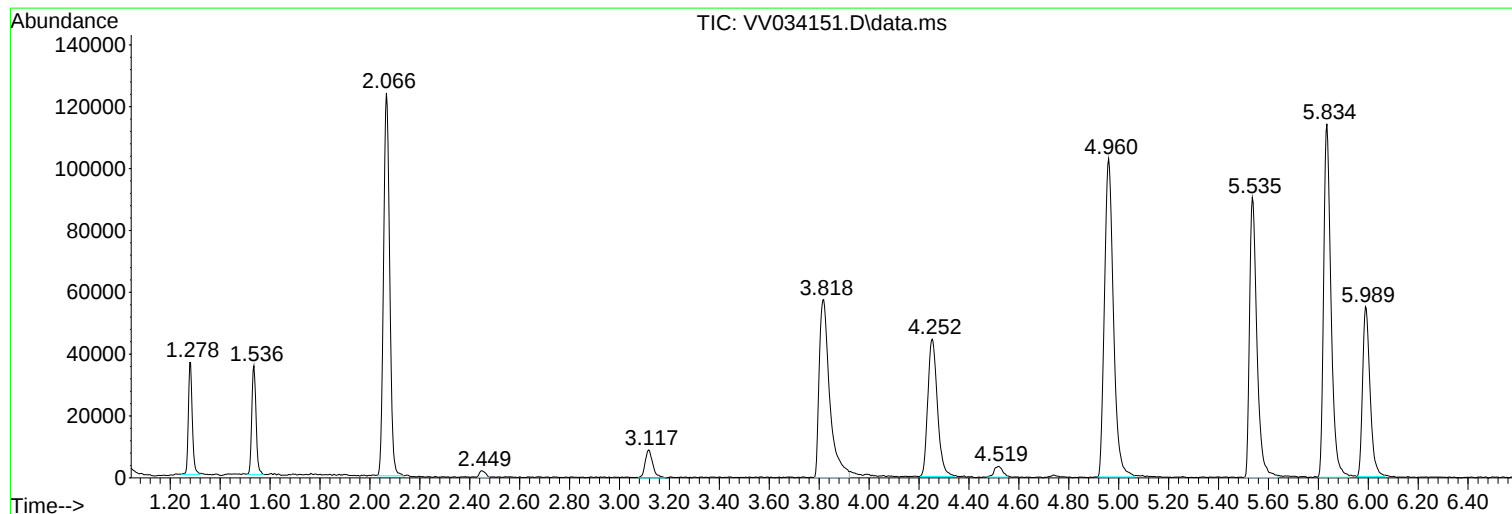

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034151.D
Acq On : 13 Feb 2024 13:35
Operator : SY/MD
Sample : P1402-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034151.D
Acq On : 13 Feb 2024 13:35
Operator : SY/MD
Sample : P1402-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc