

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034153.D
 Acq On : 13 Feb 2024 14:23
 Operator : SY/MD
 Sample : P1402-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	35560	37491	15.03%	1.702%
2	1.536	146	154	165	rBV	34518	40314	16.16%	1.830%
3	2.063	308	318	334	rBV	67790	98959	39.66%	4.493%
4	3.806	851	860	891	rBV2	21225	66091	26.49%	3.000%
5	4.249	984	998	1023	rBV	42985	112254	44.99%	5.096%
6	4.960	1204	1219	1247	rBV2	98709	249517	100.00%	11.328%
7	5.535	1388	1398	1432	rBV	92208	193390	77.51%	8.780%
8	5.838	1483	1492	1511	rBV2	22238	48299	19.36%	2.193%
9	5.989	1529	1539	1560	rBV	54424	112095	44.92%	5.089%
10	6.918	1818	1828	1850	rBV	26646	51089	20.48%	2.319%
11	7.243	1919	1929	1955	rBV	118775	217336	87.10%	9.867%
12	7.561	2020	2028	2045	rBV2	13898	26078	10.45%	1.184%
13	7.908	2118	2136	2150	rBV3	18470	34917	13.99%	1.585%
14	8.027	2164	2173	2210	rBV	90620	195216	78.24%	8.863%
15	8.786	2399	2409	2441	rBV	138417	234038	93.80%	10.625%
16	10.153	2822	2834	2850	rBV2	33930	55580	22.28%	2.523%
17	10.326	2879	2888	2894	rBV3	4086	6004	2.41%	0.273%
18	11.185	3144	3155	3175	rBV	151112	236492	94.78%	10.736%
19	11.561	3262	3272	3295	rBV	119887	187557	75.17%	8.515%




Sum of corrected areas: 2202717

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034153.D
Acq On : 13 Feb 2024 14:23
Operator : SY/MD
Sample : P1402-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

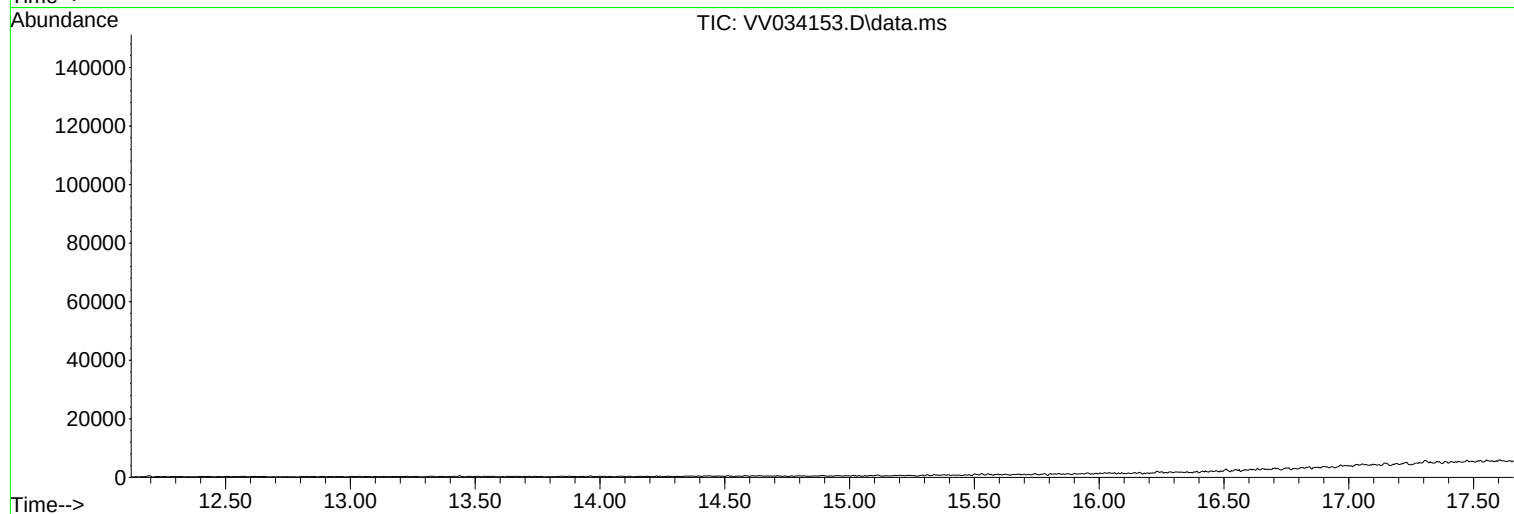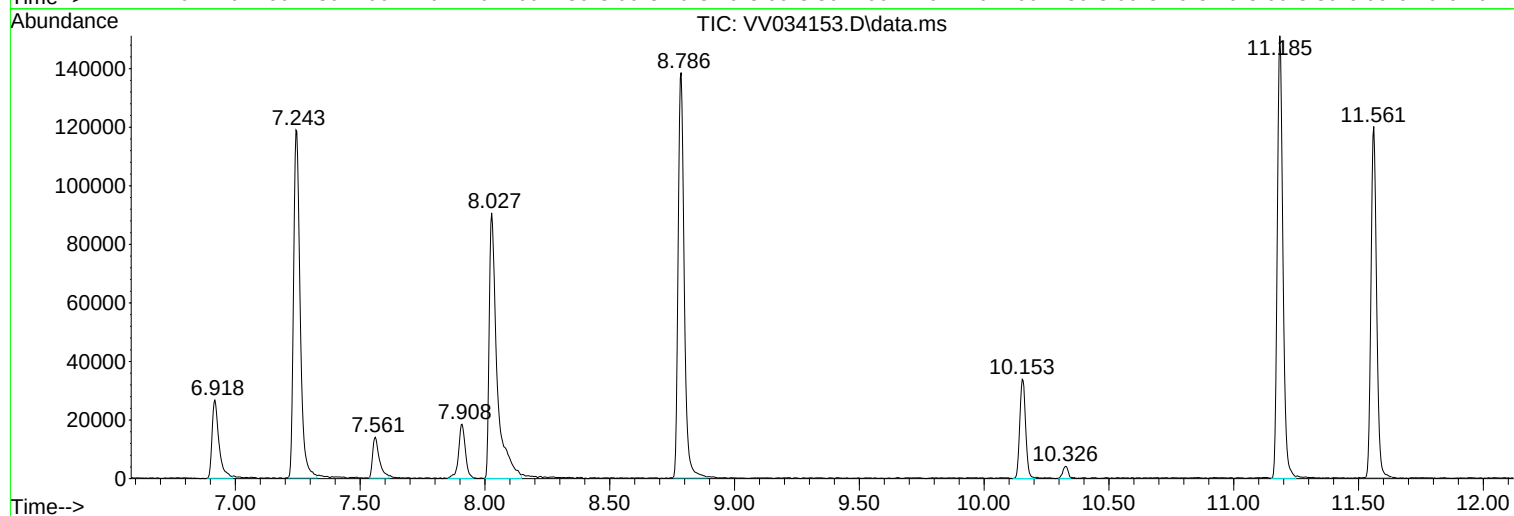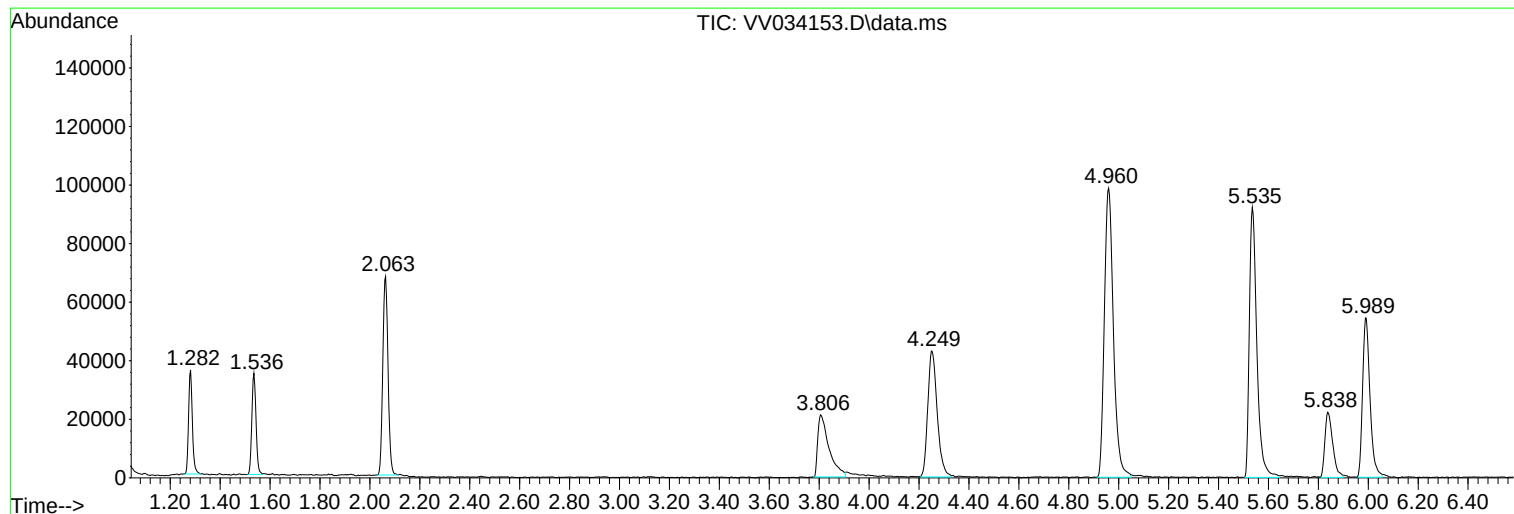

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034153.D
Acq On : 13 Feb 2024 14:23
Operator : SY/MD
Sample : P1402-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034153.D
Acq On : 13 Feb 2024 14:23
Operator : SY/MD
Sample : P1402-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc