

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034155.D
 Acq On : 13 Feb 2024 15:10
 Operator : SY/MD
 Sample : P1455-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.192	43	47	53	rBV2	3629	3372	1.34%	0.140%
2	1.282	66	75	83	rBV	38210	39904	15.91%	1.652%
3	1.536	146	154	165	rBV	33800	39941	15.93%	1.653%
4	2.063	308	318	331	rBV	71582	107152	42.73%	4.436%
5	3.822	856	865	901	rBV2	18913	73042	29.13%	3.024%
6	4.256	980	1000	1023	rBV3	45147	130598	52.08%	5.406%
7	4.735	1134	1149	1172	rBV3	32615	81673	32.57%	3.381%
8	4.960	1205	1219	1249	rBV3	98915	249773	99.60%	10.340%
9	5.535	1387	1398	1429	rBV	101589	208858	83.28%	8.646%
10	5.841	1484	1493	1513	rVB3	11084	23590	9.41%	0.977%
11	5.989	1526	1539	1565	rBV	52916	112978	45.05%	4.677%
12	6.918	1819	1828	1849	rBV	25463	50813	20.26%	2.104%
13	7.243	1915	1929	1954	rBV	121497	218683	87.20%	9.053%
14	7.561	2019	2028	2048	rBV3	13553	27328	10.90%	1.131%
15	7.905	2123	2135	2156	rVB	69070	117764	46.96%	4.875%
16	8.030	2165	2174	2214	rBV	89183	195642	78.01%	8.099%
17	8.786	2399	2409	2433	rBV	149776	250786	100.00%	10.382%
18	10.153	2824	2834	2845	rBV2	33467	51959	20.72%	2.151%
19	11.185	3144	3155	3181	rBV	158249	249212	99.37%	10.317%
20	11.561	3261	3272	3295	rBV	115461	182560	72.80%	7.557%




Sum of corrected areas: 2415628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034155.D
Acq On : 13 Feb 2024 15:10
Operator : SY/MD
Sample : P1455-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

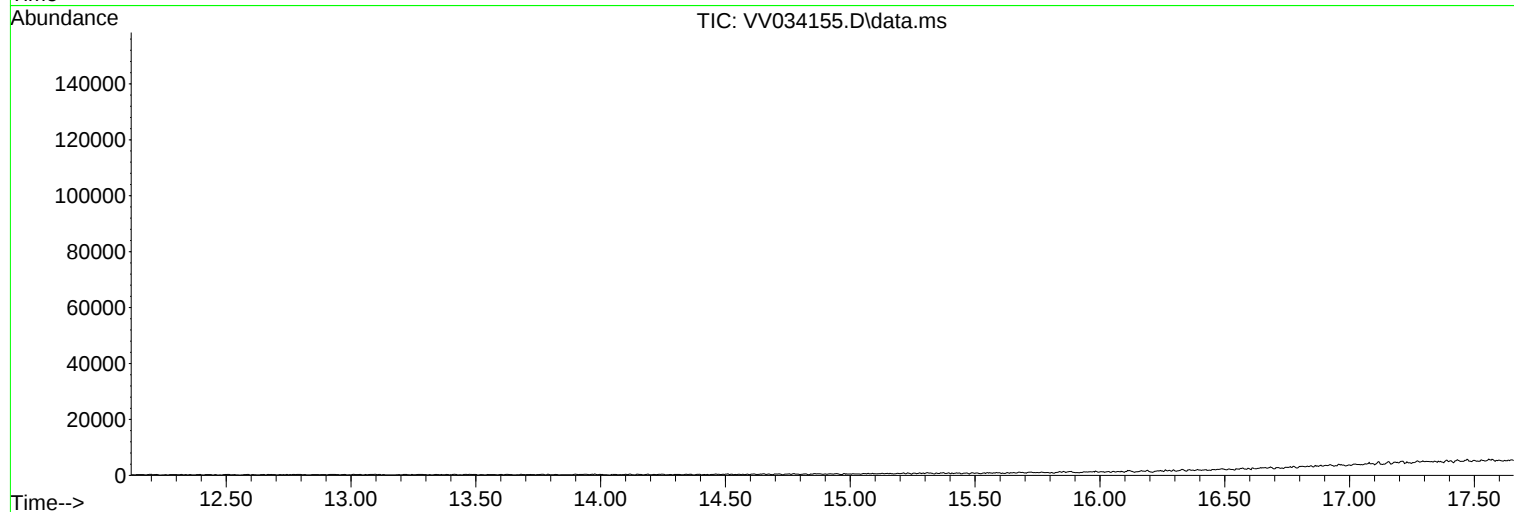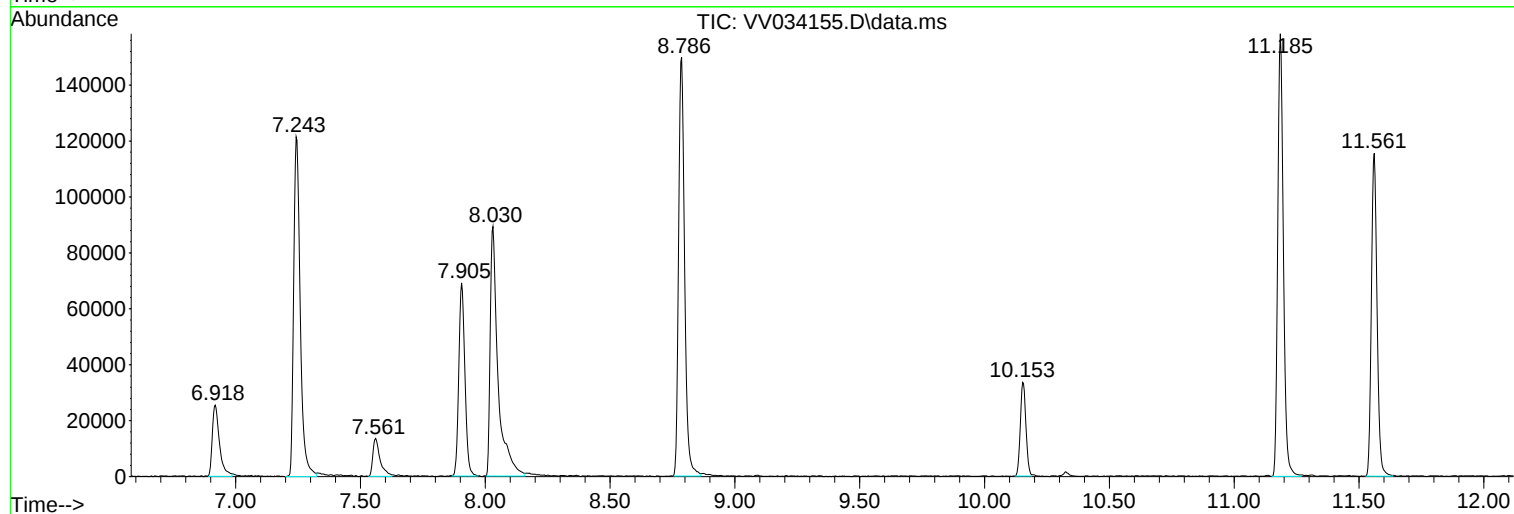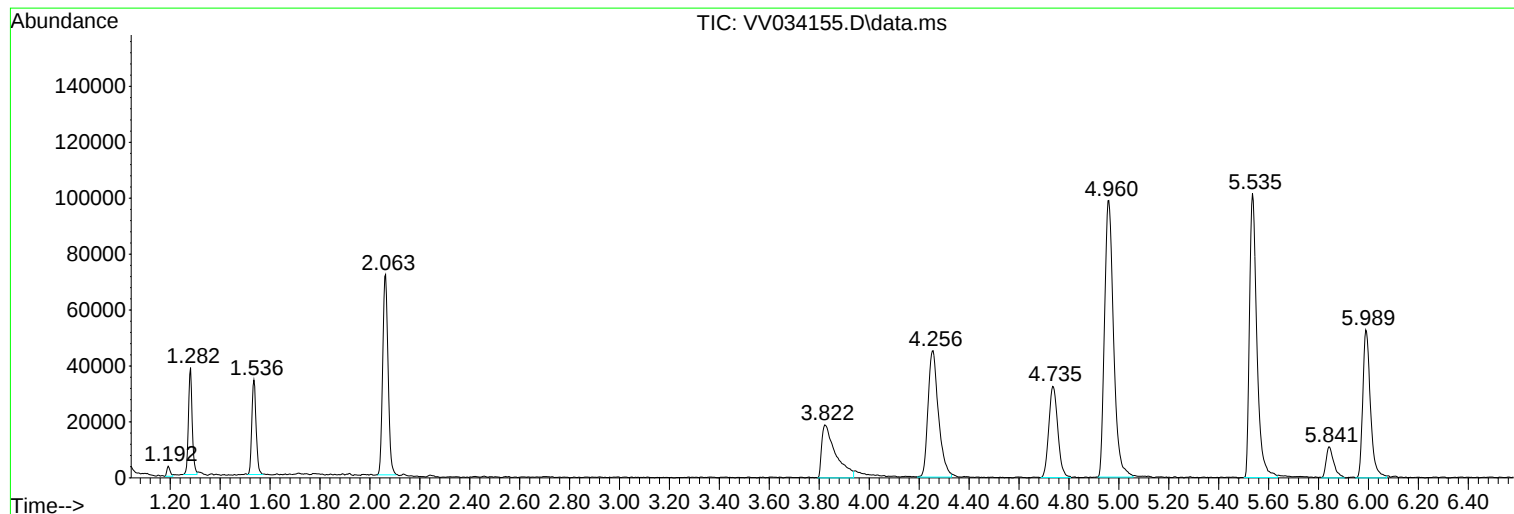

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034155.D
Acq On : 13 Feb 2024 15:10
Operator : SY/MD
Sample : P1455-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034155.D
Acq On : 13 Feb 2024 15:10
Operator : SY/MD
Sample : P1455-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
