

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034156.D
 Acq On : 13 Feb 2024 15:34
 Operator : SY/MD
 Sample : P1455-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	65	75	88	rBV	33406	36645	5.90%	1.176%
2	1.536	145	154	168	rBV	31902	37921	6.10%	1.217%
3	2.066	308	319	336	rBV3	113660	192649	31.01%	6.183%
4	3.114	635	645	661	rBV2	5614	11839	1.91%	0.380%
5	3.818	853	864	895	rBV3	47218	133027	21.42%	4.270%
6	4.252	984	999	1025	rBV2	41591	114008	18.35%	3.659%
7	4.738	1135	1150	1167	rVB3	11127	27928	4.50%	0.896%
8	4.960	1204	1219	1244	rBV2	92519	232148	37.37%	7.451%
9	5.535	1388	1398	1437	rBV	92005	195363	31.45%	6.270%
10	5.831	1476	1490	1525	rBV	310718	621169	100.00%	19.937%
11	5.989	1528	1539	1557	rBV3	49962	102298	16.47%	3.283%
12	6.918	1819	1828	1850	rBV2	24521	47343	7.62%	1.520%
13	7.243	1919	1929	1961	rBV	111221	202103	32.54%	6.487%
14	7.561	2020	2028	2045	rBV2	13291	25920	4.17%	0.832%
15	7.905	2123	2135	2156	rBV	147619	248693	40.04%	7.982%
16	8.027	2165	2173	2206	rBV	82949	182584	29.39%	5.860%
17	8.783	2398	2408	2440	rBV	137470	234743	37.79%	7.534%
18	10.153	2821	2834	2849	rBV	32697	52281	8.42%	1.678%
19	11.185	3144	3155	3178	rBV	152357	240791	38.76%	7.728%
20	11.561	3261	3272	3296	rBV	112140	176183	28.36%	5.655%




Sum of corrected areas: 3115636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034156.D
Acq On : 13 Feb 2024 15:34
Operator : SY/MD
Sample : P1455-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

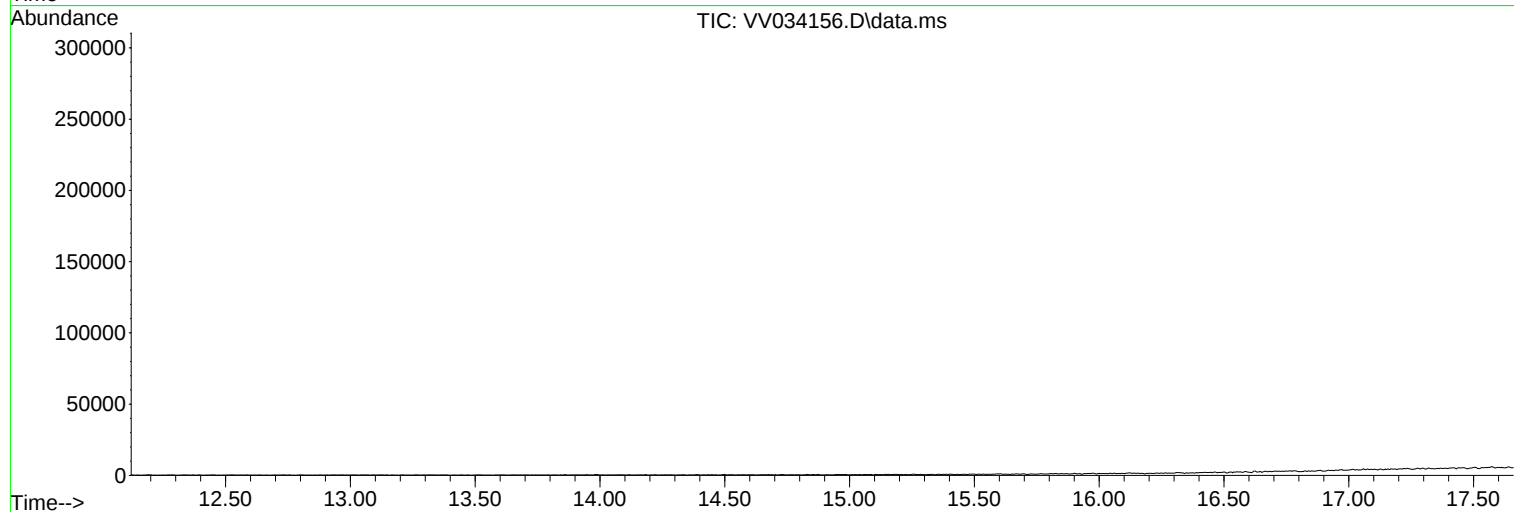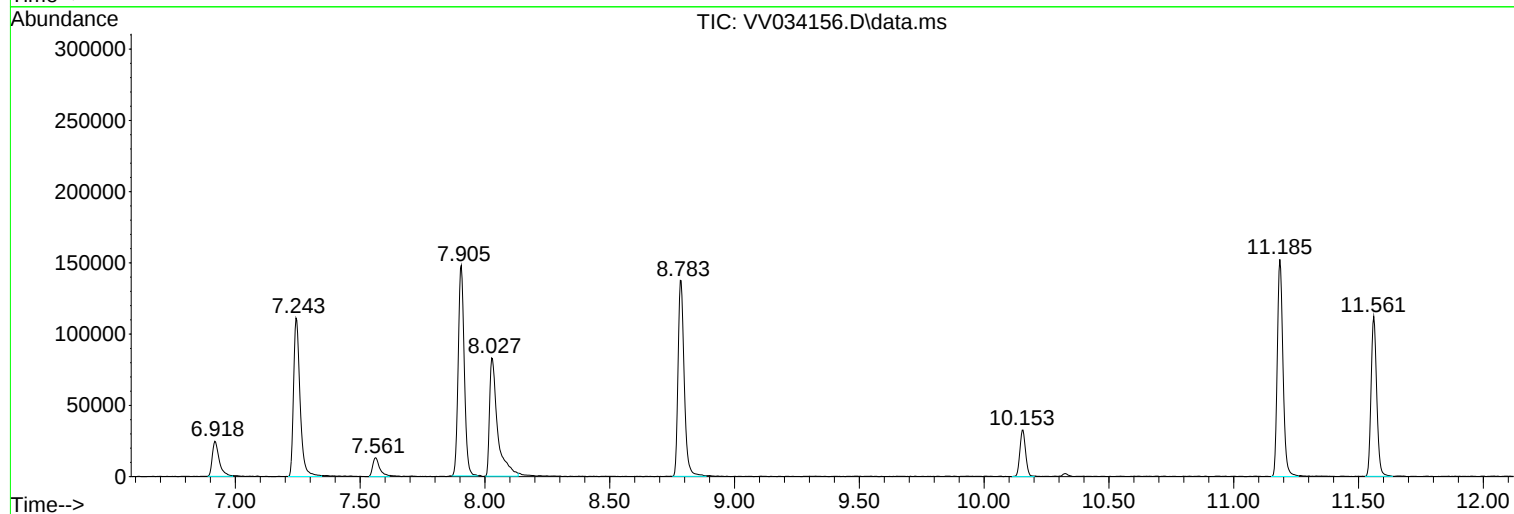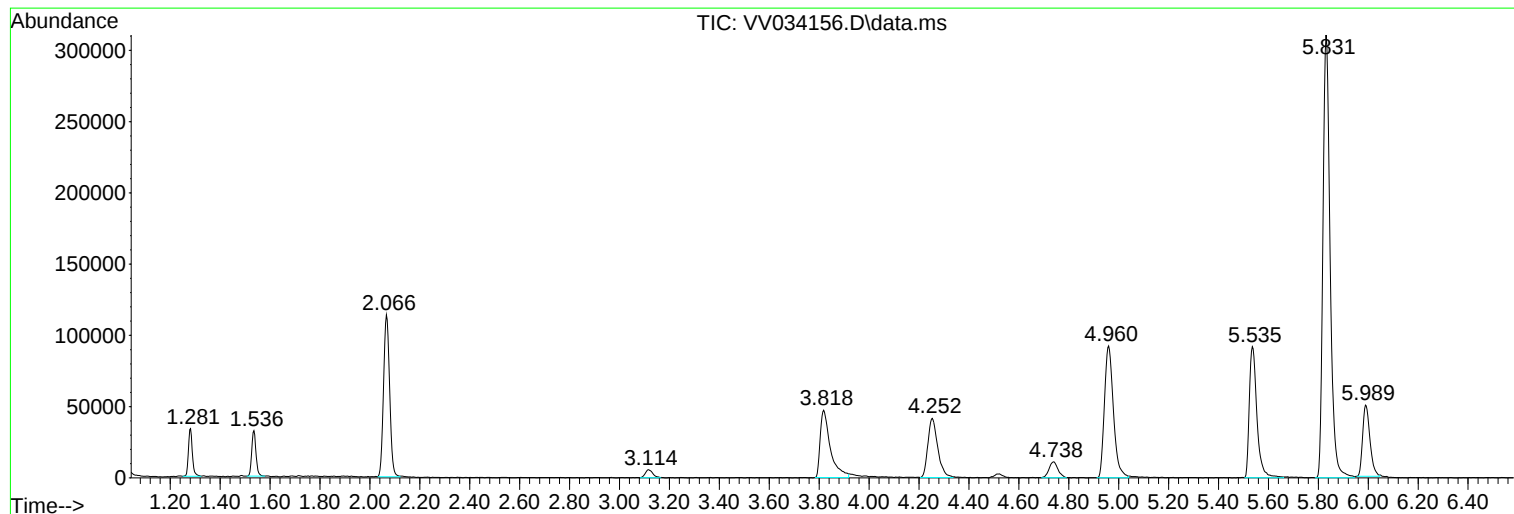

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034156.D
Acq On : 13 Feb 2024 15:34
Operator : SY/MD
Sample : P1455-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034156.D
Acq On : 13 Feb 2024 15:34
Operator : SY/MD
Sample : P1455-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
