

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034160.D
 Acq On : 13 Feb 2024 18:20
 Operator : SY/MD
 Sample : P1402-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	64	74	89	rBV2	38650	51753	21.29%	2.499%
2	1.535	146	154	167	rVB	33001	39204	16.13%	1.893%
3	2.060	306	317	335	rBV	67421	98816	40.65%	4.771%
4	3.600	786	796	812	rBV4	3867	8682	3.57%	0.419%
5	3.828	858	867	902	rBV2	13954	64813	26.66%	3.129%
6	4.252	983	999	1026	rBV2	41855	109618	45.10%	5.293%
7	4.960	1205	1219	1245	rBV2	97342	243075	100.00%	11.737%
8	5.535	1387	1398	1423	rBV	88503	185047	76.13%	8.935%
9	5.992	1526	1540	1567	rBV2	52899	112447	46.26%	5.429%
10	6.464	1678	1687	1697	rBV6	2172	4224	1.74%	0.204%
11	6.918	1817	1828	1852	rBV2	25434	50496	20.77%	2.438%
12	7.243	1918	1929	1953	rBV	117010	213929	88.01%	10.329%
13	7.561	2018	2028	2052	rBV2	13784	26344	10.84%	1.272%
14	8.030	2166	2174	2188	rBV	84402	163819	67.39%	7.910%
15	8.786	2395	2409	2433	rBV	133207	223365	91.89%	10.785%
16	10.152	2823	2834	2848	rBV	32875	52828	21.73%	2.551%
17	10.889	3056	3063	3071	rBV5	2269	4102	1.69%	0.198%
18	11.185	3145	3155	3175	rBV	145007	226015	92.98%	10.913%
19	11.561	3261	3272	3296	rBV	117241	185603	76.36%	8.962%
20	12.294	3494	3500	3512	rVB4	4299	6900	2.84%	0.333%




Sum of corrected areas: 2071080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

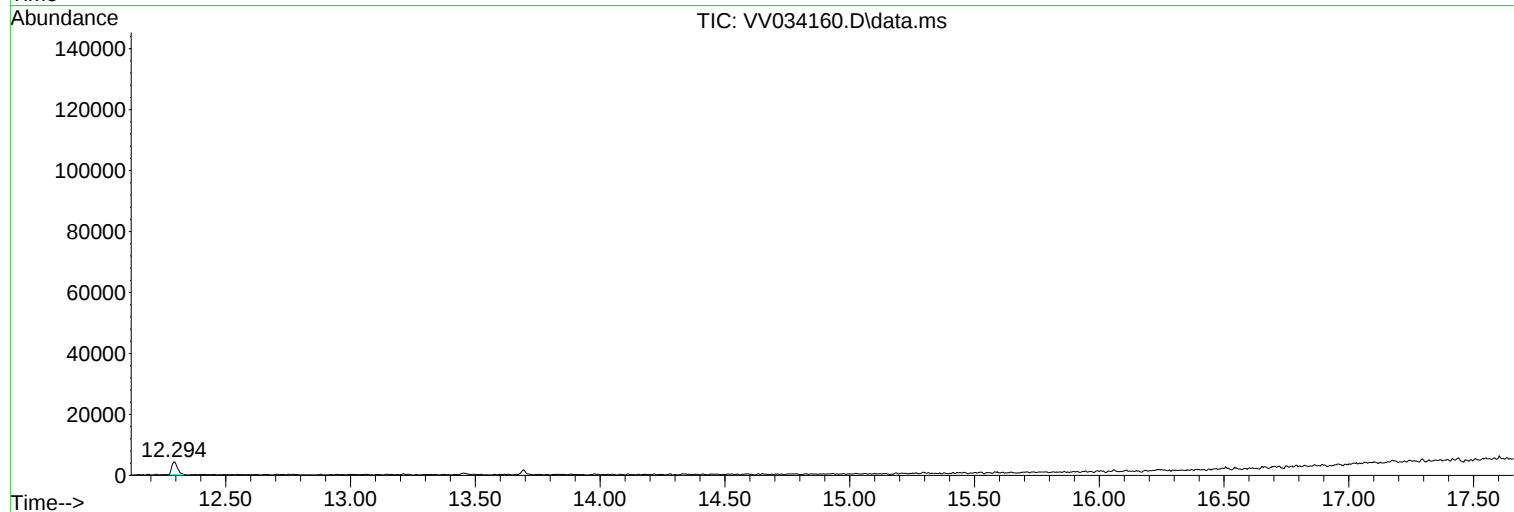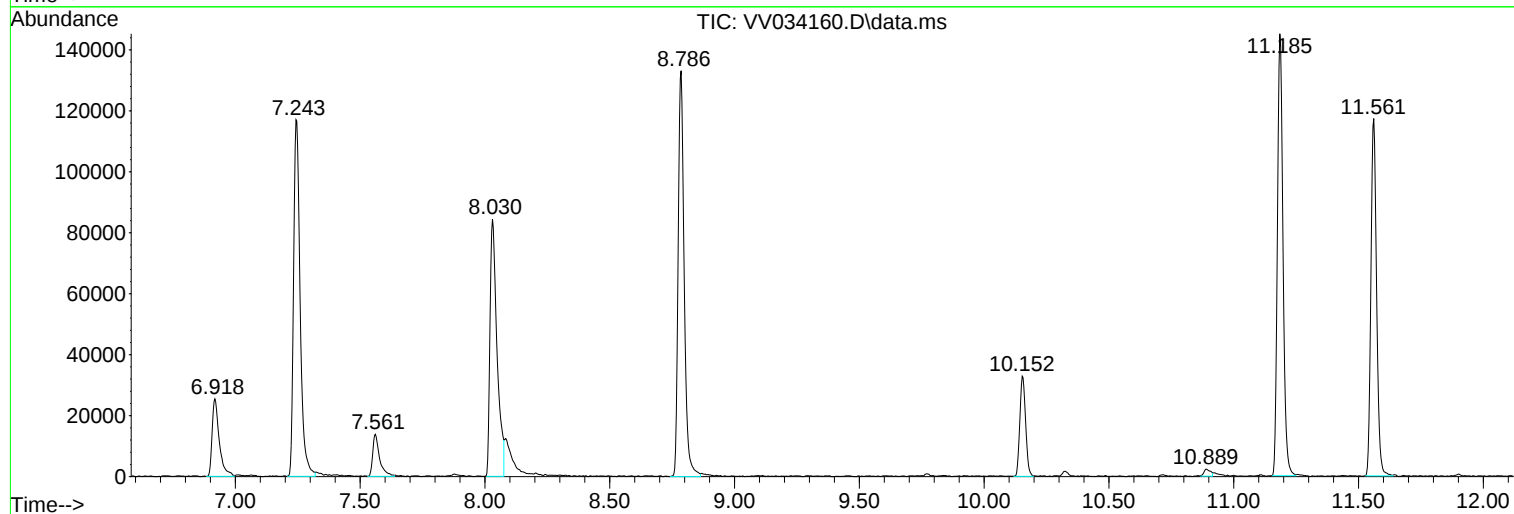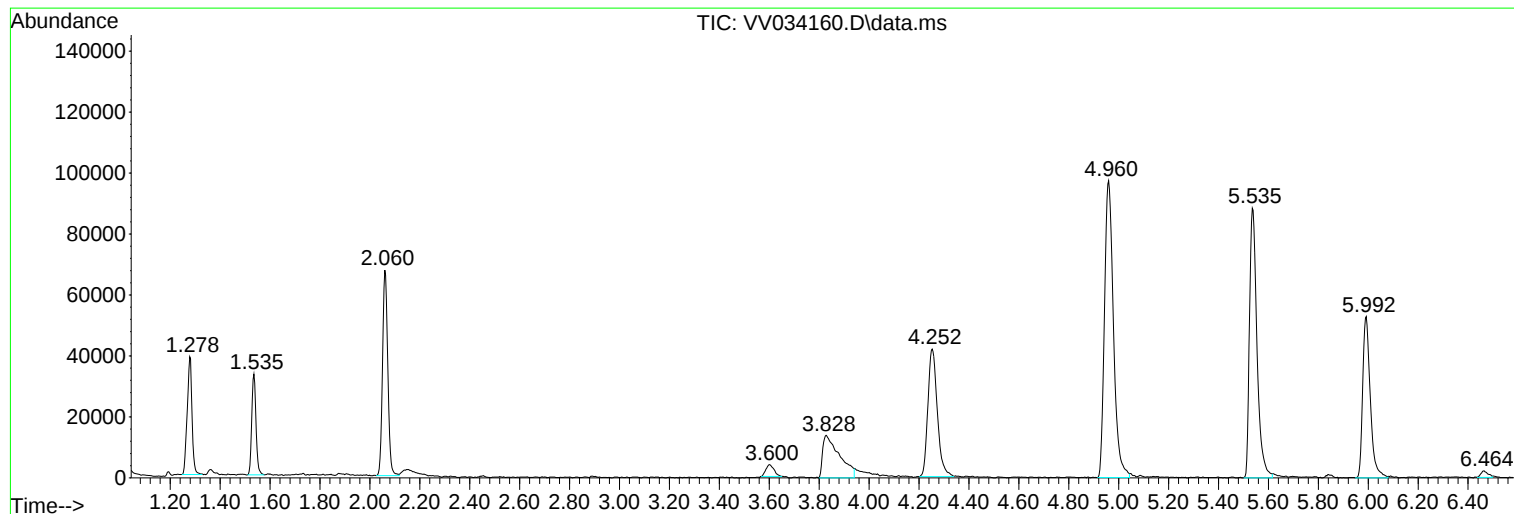

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034160.D
Acq On : 13 Feb 2024 18:20
Operator : SY/MD
Sample : P1402-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc