

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034162.D
 Acq On : 13 Feb 2024 19:07
 Operator : SY/MD
 Sample : P1455-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	65	75	86	rBV	32120	34803	5.52%	0.942%
2	1.535	146	154	167	rVB	31455	36326	5.76%	0.984%
3	2.069	308	320	346	rVB3	209621	344902	54.71%	9.339%
4	3.117	633	646	665	rBV2	18517	39869	6.32%	1.079%
5	3.815	851	863	897	rBV2	105986	274183	43.49%	7.424%
6	4.252	983	999	1027	rBV2	41944	114365	18.14%	3.097%
7	4.513	1063	1080	1098	rVB3	8340	20770	3.29%	0.562%
8	4.738	1134	1150	1168	rVB2	9277	22555	3.58%	0.611%
9	4.960	1205	1219	1246	rBV3	92386	233669	37.06%	6.327%
10	5.535	1388	1398	1422	rBV	87460	178979	28.39%	4.846%
11	5.831	1478	1490	1529	rBV	268833	534084	84.71%	14.461%
12	5.992	1529	1540	1564	rVB	50826	105174	16.68%	2.848%
13	6.918	1818	1828	1847	rBV2	24371	46516	7.38%	1.259%
14	7.246	1917	1930	1960	rBV2	111673	203702	32.31%	5.515%
15	7.561	2017	2028	2042	rBV2	12960	23634	3.75%	0.640%
16	7.905	2122	2135	2154	rBV	376600	630462	100.00%	17.070%
17	8.027	2165	2173	2221	rBV	84594	181243	28.75%	4.907%
18	8.786	2399	2409	2436	rBV	132800	219560	34.83%	5.945%
19	10.152	2824	2834	2849	rBV	31958	49896	7.91%	1.351%
20	11.185	3142	3155	3176	rBV	141373	221689	35.16%	6.002%
21	11.561	3261	3272	3296	rBV	111127	176909	28.06%	4.790%




Sum of corrected areas: 3693290

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034162.D
Acq On : 13 Feb 2024 19:07
Operator : SY/MD
Sample : P1455-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

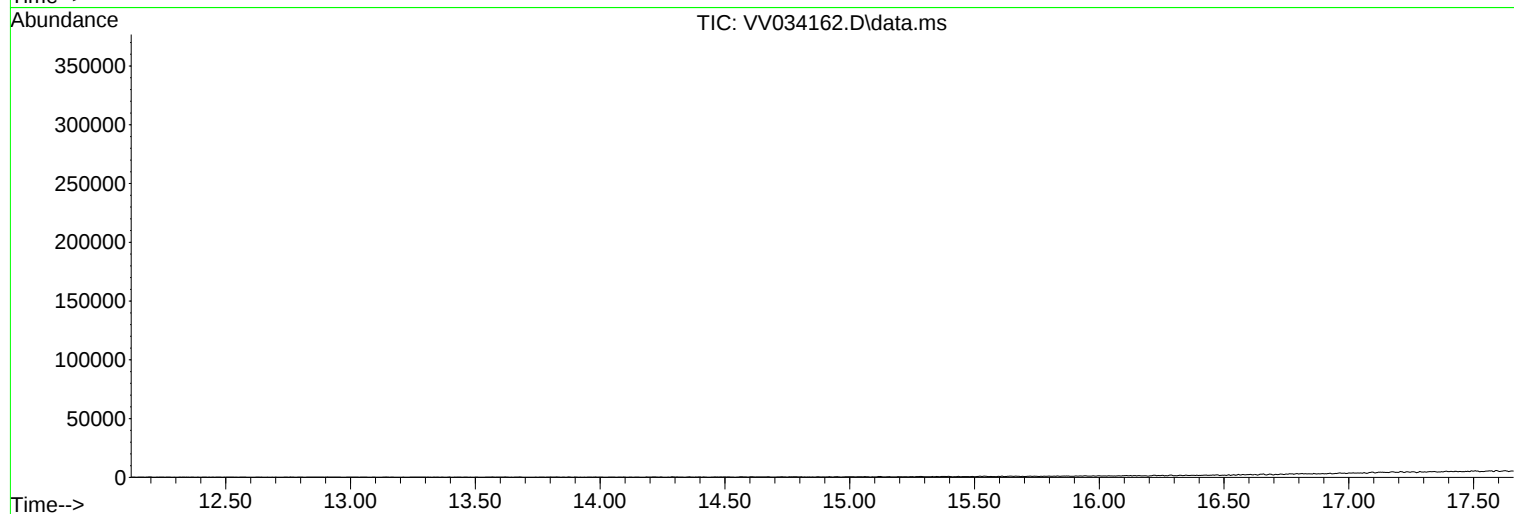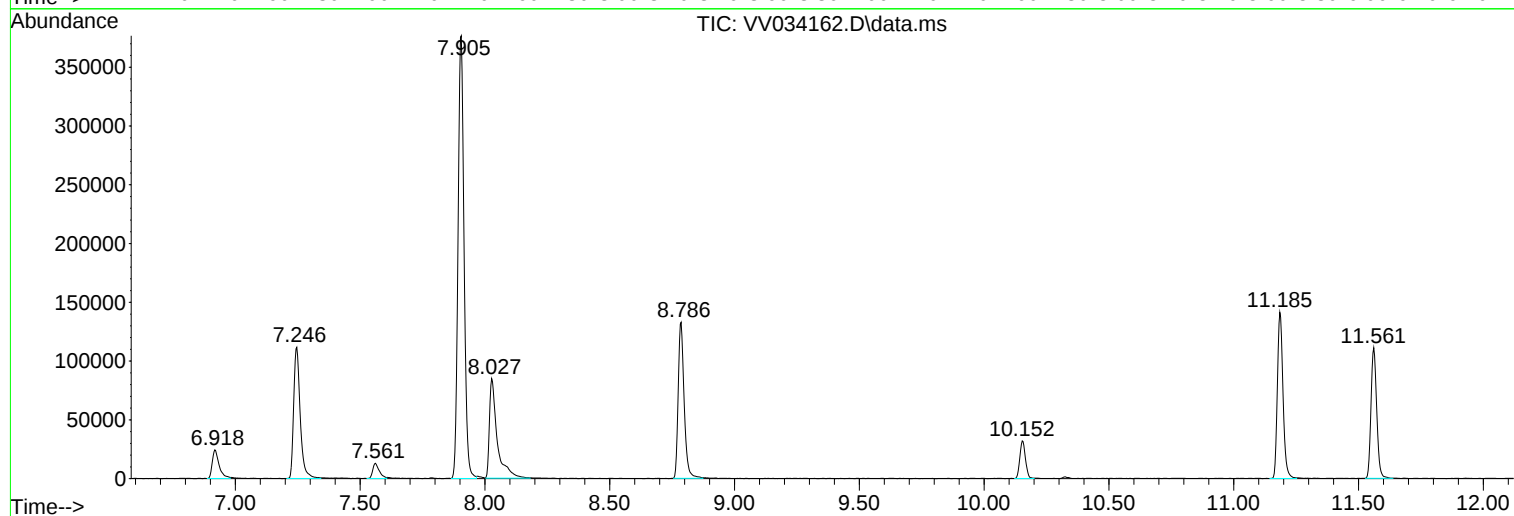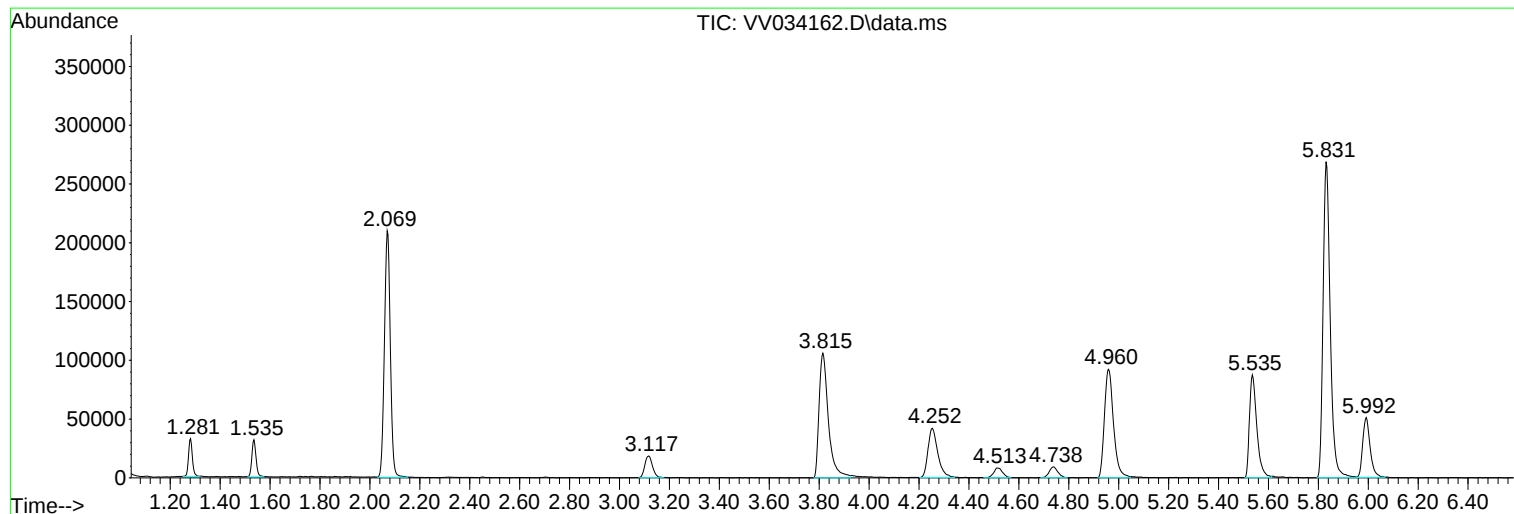

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034162.D
Acq On : 13 Feb 2024 19:07
Operator : SY/MD
Sample : P1455-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034162.D
Acq On : 13 Feb 2024 19:07
Operator : SY/MD
Sample : P1455-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------