

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
 Data File : VV034163.D
 Acq On : 13 Feb 2024 19:31
 Operator : SY/MD
 Sample : P1455-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rBV	34936	36195	15.42%	1.544%
2	1.536	146	154	166	rVB	31398	36170	15.41%	1.543%
3	2.063	308	318	335	rVB2	66203	99839	42.53%	4.260%
4	3.815	852	863	894	rBV3	22256	74001	31.53%	3.157%
5	4.252	984	999	1026	rBV3	43459	128014	54.54%	5.462%
6	4.738	1134	1150	1172	rBV2	45672	113668	48.42%	4.850%
7	4.960	1204	1219	1245	rBV4	92656	234735	100.00%	10.016%
8	5.535	1387	1398	1428	rBV	87588	181167	77.18%	7.730%
9	5.841	1483	1493	1512	rBV2	21516	44604	19.00%	1.903%
10	5.992	1528	1540	1568	rBV	50812	108481	46.21%	4.629%
11	6.918	1819	1828	1848	rBV2	24200	45695	19.47%	1.950%
12	7.243	1918	1929	1956	rBV	114030	207668	88.47%	8.861%
13	7.561	2019	2028	2044	rBV2	13280	25127	10.70%	1.072%
14	7.905	2120	2135	2154	rBV	106957	182013	77.54%	7.766%
15	8.027	2162	2173	2188	rBV	82818	159245	67.84%	6.795%
16	8.786	2398	2409	2432	rBV	130305	219271	93.41%	9.356%
17	10.153	2825	2834	2847	rBV2	32306	50585	21.55%	2.158%
18	11.185	3145	3155	3182	rBV	138599	220309	93.85%	9.400%
19	11.561	3262	3272	3297	rBV	111356	176886	75.36%	7.547%




Sum of corrected areas: 2343673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034163.D
Acq On : 13 Feb 2024 19:31
Operator : SY/MD
Sample : P1455-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

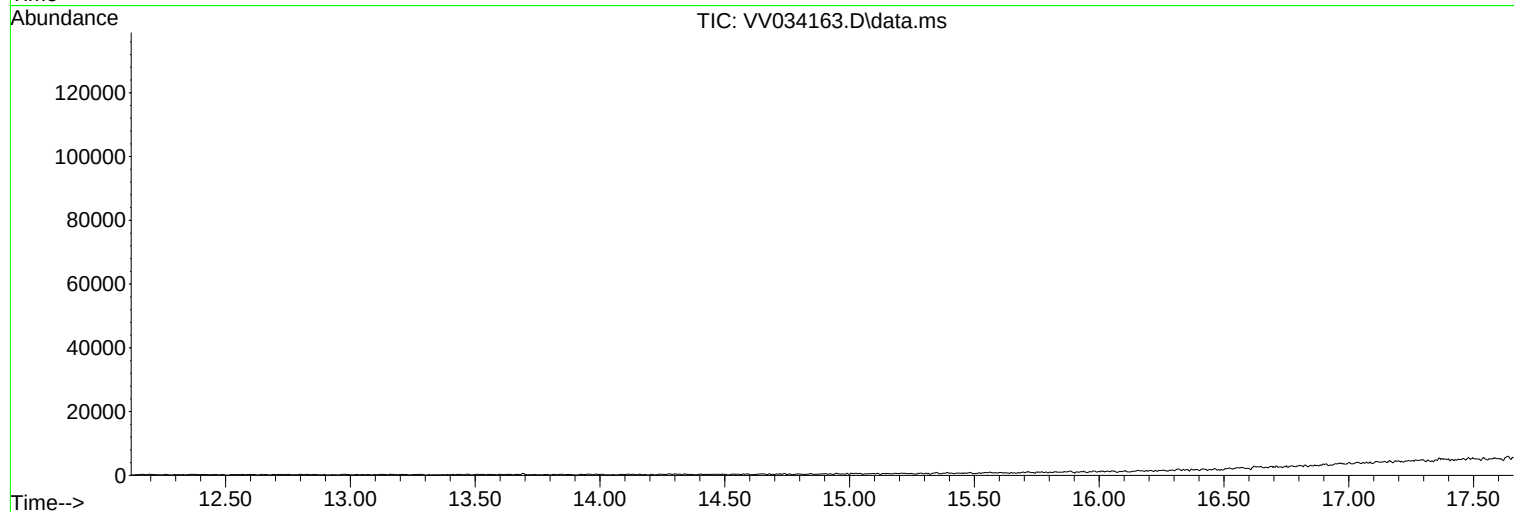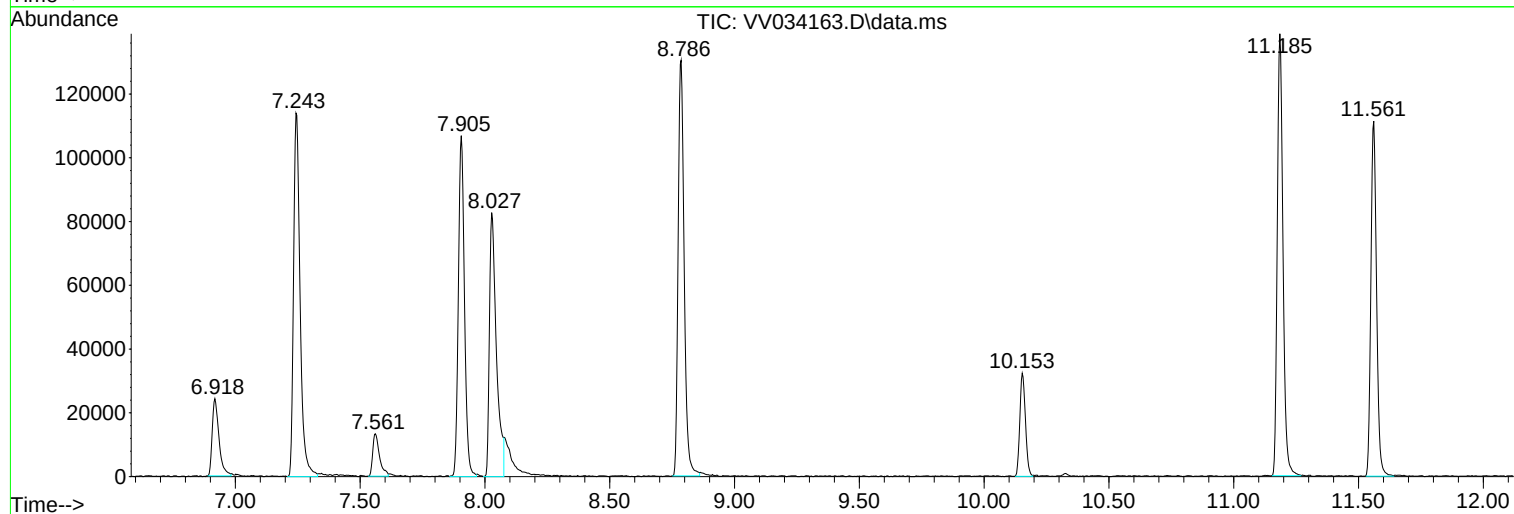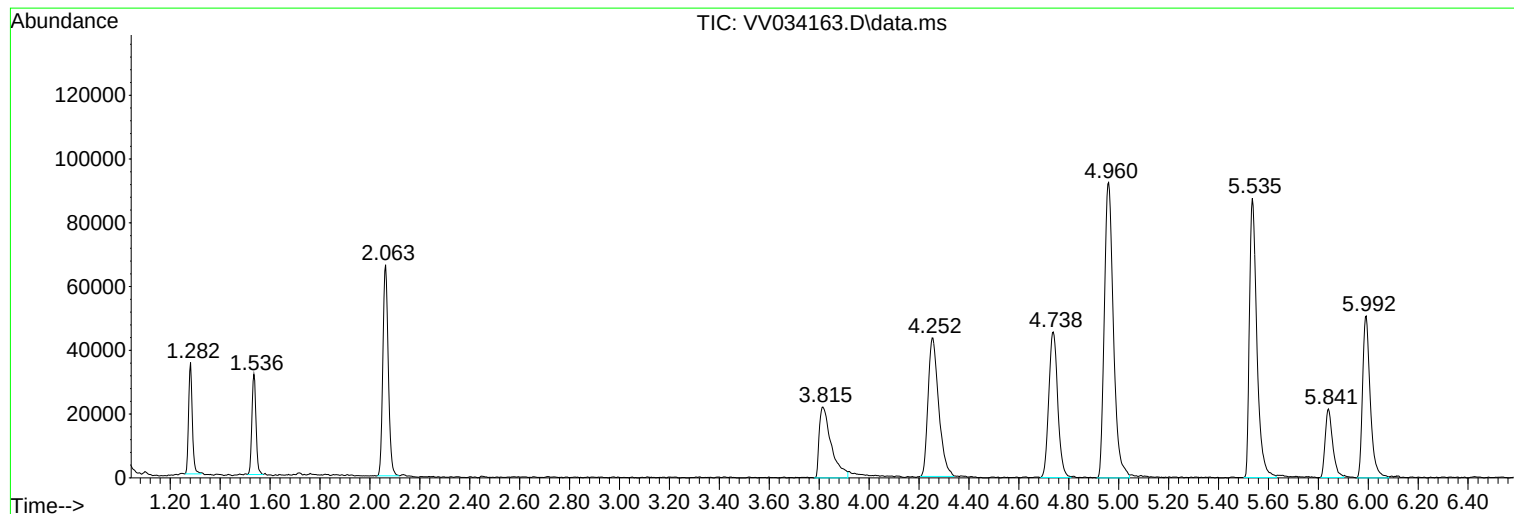

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034163.D
Acq On : 13 Feb 2024 19:31
Operator : SY/MD
Sample : P1455-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021324\
Data File : VV034163.D
Acq On : 13 Feb 2024 19:31
Operator : SY/MD
Sample : P1455-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
