

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024644.D
 Acq On : 14 Feb 2022 12:21
 Operator : SY/MD
 Sample : VV0214WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK304

Quant Time: Feb 15 06:26:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 15 06:26:19 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	158983	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	159822	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	79730	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	67977	5.101	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 102.000%		
7) Chloroethane-d5	1.571	69	62897	5.583	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 111.600%		
11) 1,1-Dichloroethene-d2	2.111	63	111490	3.825	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 76.400%		
20) 2-Butanone-d5	3.905	46	131011	59.219	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 118.440%		
24) Chloroform-d	4.352	84	129373	5.516	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 110.400%		
26) 1,2-Dichloroethane-d4	5.034	65	63760	5.991	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 119.800%		
32) Benzene-d6	5.050	84	271112	5.979	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 119.600%		
36) 1,2-Dichloropropane-d6	6.069	67	80453	5.704	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 114.000%		
41) Toluene-d8	7.317	98	246816	5.836	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 116.800%		
43) trans-1,3-Dichloroprop...	7.622	79	29385	5.159	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 103.200%		
46) 2-Hexanone-d5	8.088	63	110598	55.116	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 110.240%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46208	5.503	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 110.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	74927	5.830	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 116.600%		
Target Compounds						
25) Chloroform	4.384	83	2845	0.097	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024644.D
Acq On : 14 Feb 2022 12:21
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK304

Quant Time: Feb 15 06:26:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

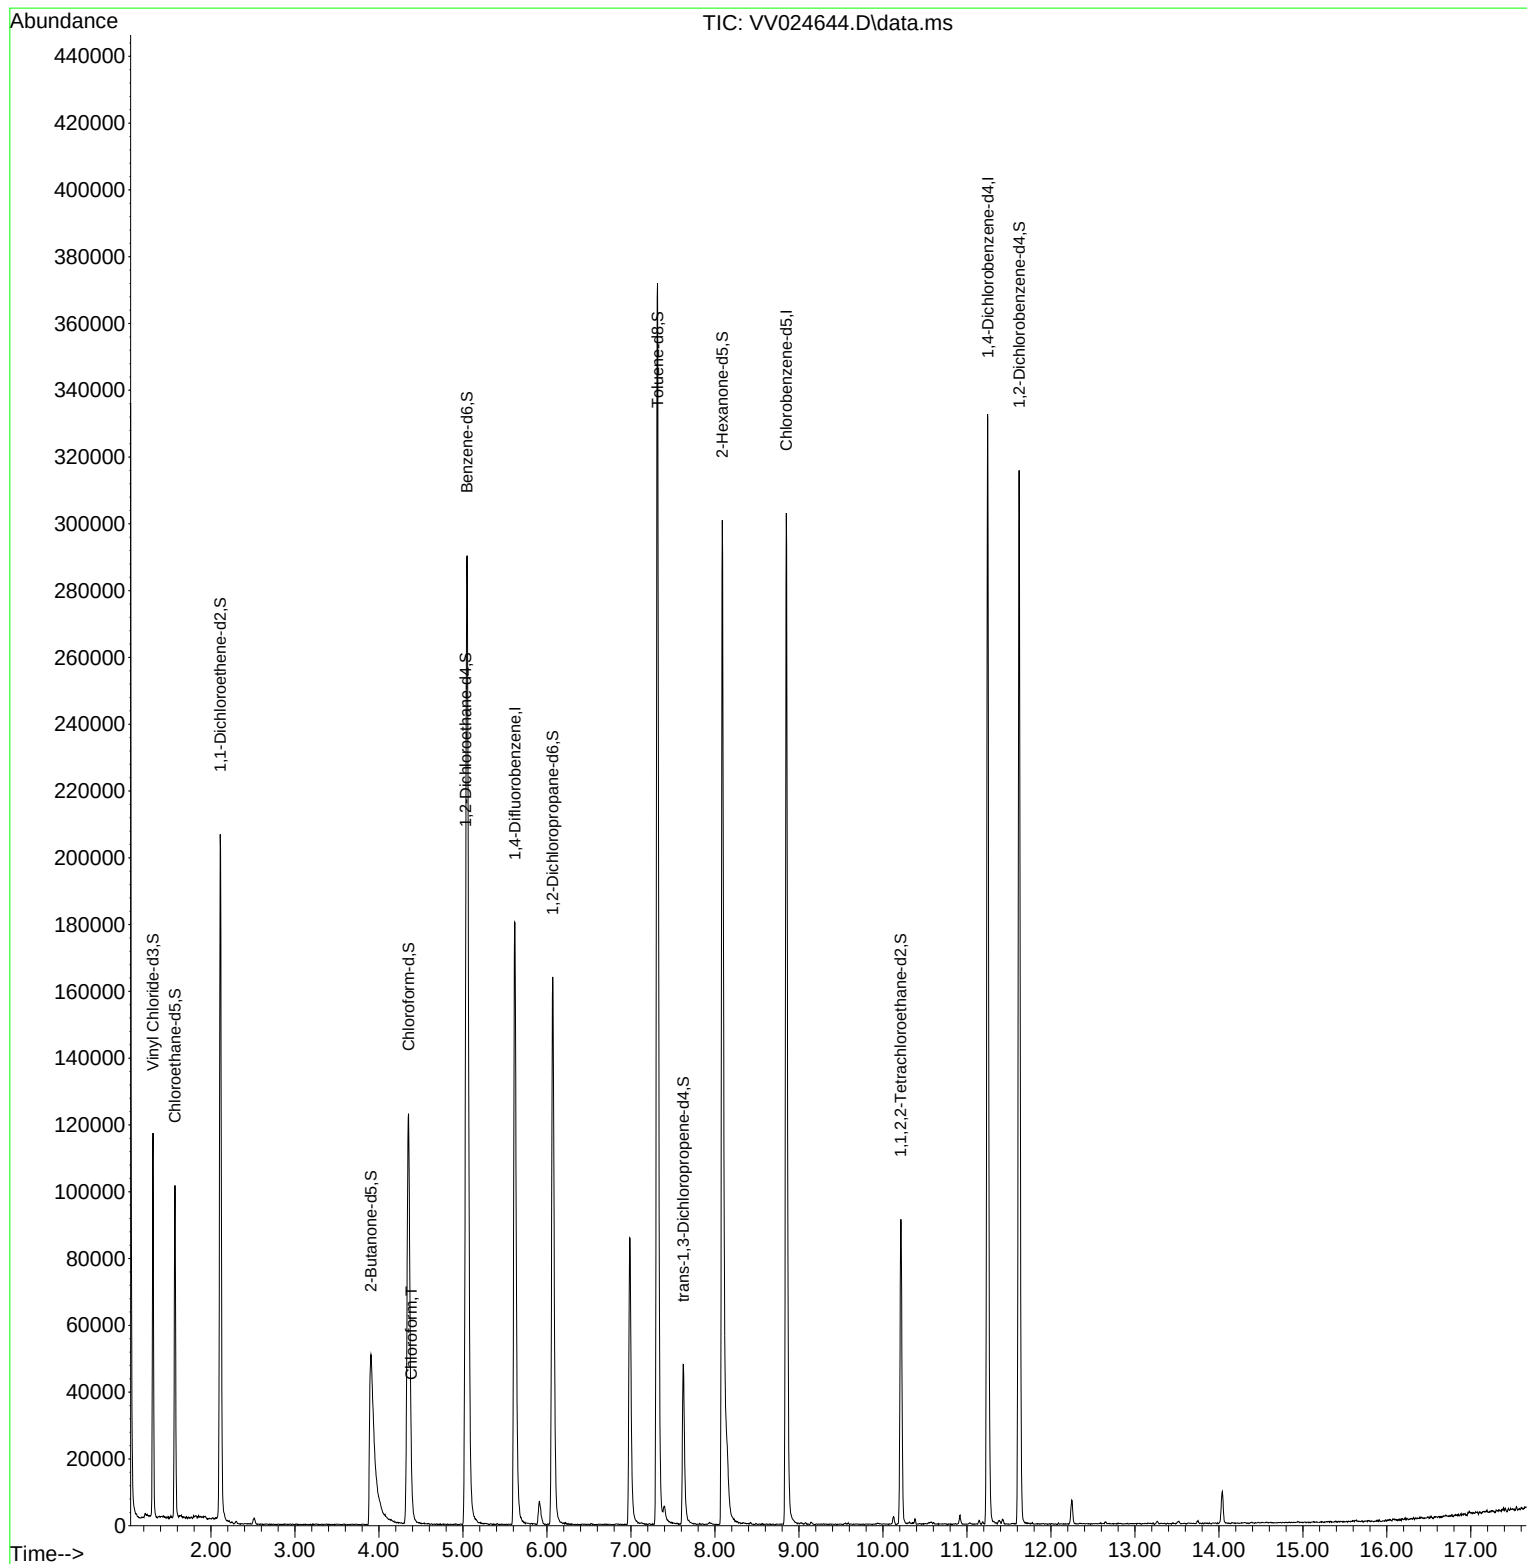

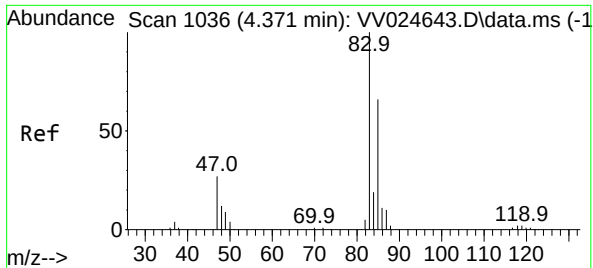

#25
Chloroform
Concen: 0.097 ug/L
RT: 4.384 min Scan# 10
Delta R.T. 0.013 min
Lab File: VV024644.D
Acq: 14 Feb 2022 12:21

Instrument :
MSVOA_V
ClientSampleId :
VBLK304

Tgt Ion: 83 Resp: 2845
Ion Ratio Lower Upper
83 100
85 79.3 45.2 84.0

