

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024645.D
 Acq On : 14 Feb 2022 12:56
 Operator : SY/MD
 Sample : N1479-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 15 06:27:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 15 06:26:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	117476	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	116058	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	57867	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	49788	5.056	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.200%	
7) Chloroethane-d5	1.568	69	46020	5.528	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	110.600%	
11) 1,1-Dichloroethene-d2	2.108	63	81200	3.770	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.400%	
20) 2-Butanone-d5	3.908	46	85229	52.137	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.280%	
24) Chloroform-d	4.346	84	93377	5.388	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.800%	
26) 1,2-Dichloroethane-d4	5.031	65	45661	5.806	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	116.200%	
32) Benzene-d6	5.047	84	193384	5.873	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	117.400%	
36) 1,2-Dichloropropane-d6	6.066	67	59019	5.763	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.200%	
41) Toluene-d8	7.313	98	175025	5.699	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	114.000%	
43) trans-1,3-Dichloroprop...	7.622	79	20829	5.036	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	100.800%	
46) 2-Hexanone-d5	8.088	63	76900	52.774	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.540%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32594	5.345	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53554	5.741	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.800%	
Target Compounds					Qvalue	
25) Chloroform	4.375	83	2735	0.127	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024645.D
Acq On : 14 Feb 2022 12:56
Operator : SY/MD
Sample : N1479-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 15 06:27:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

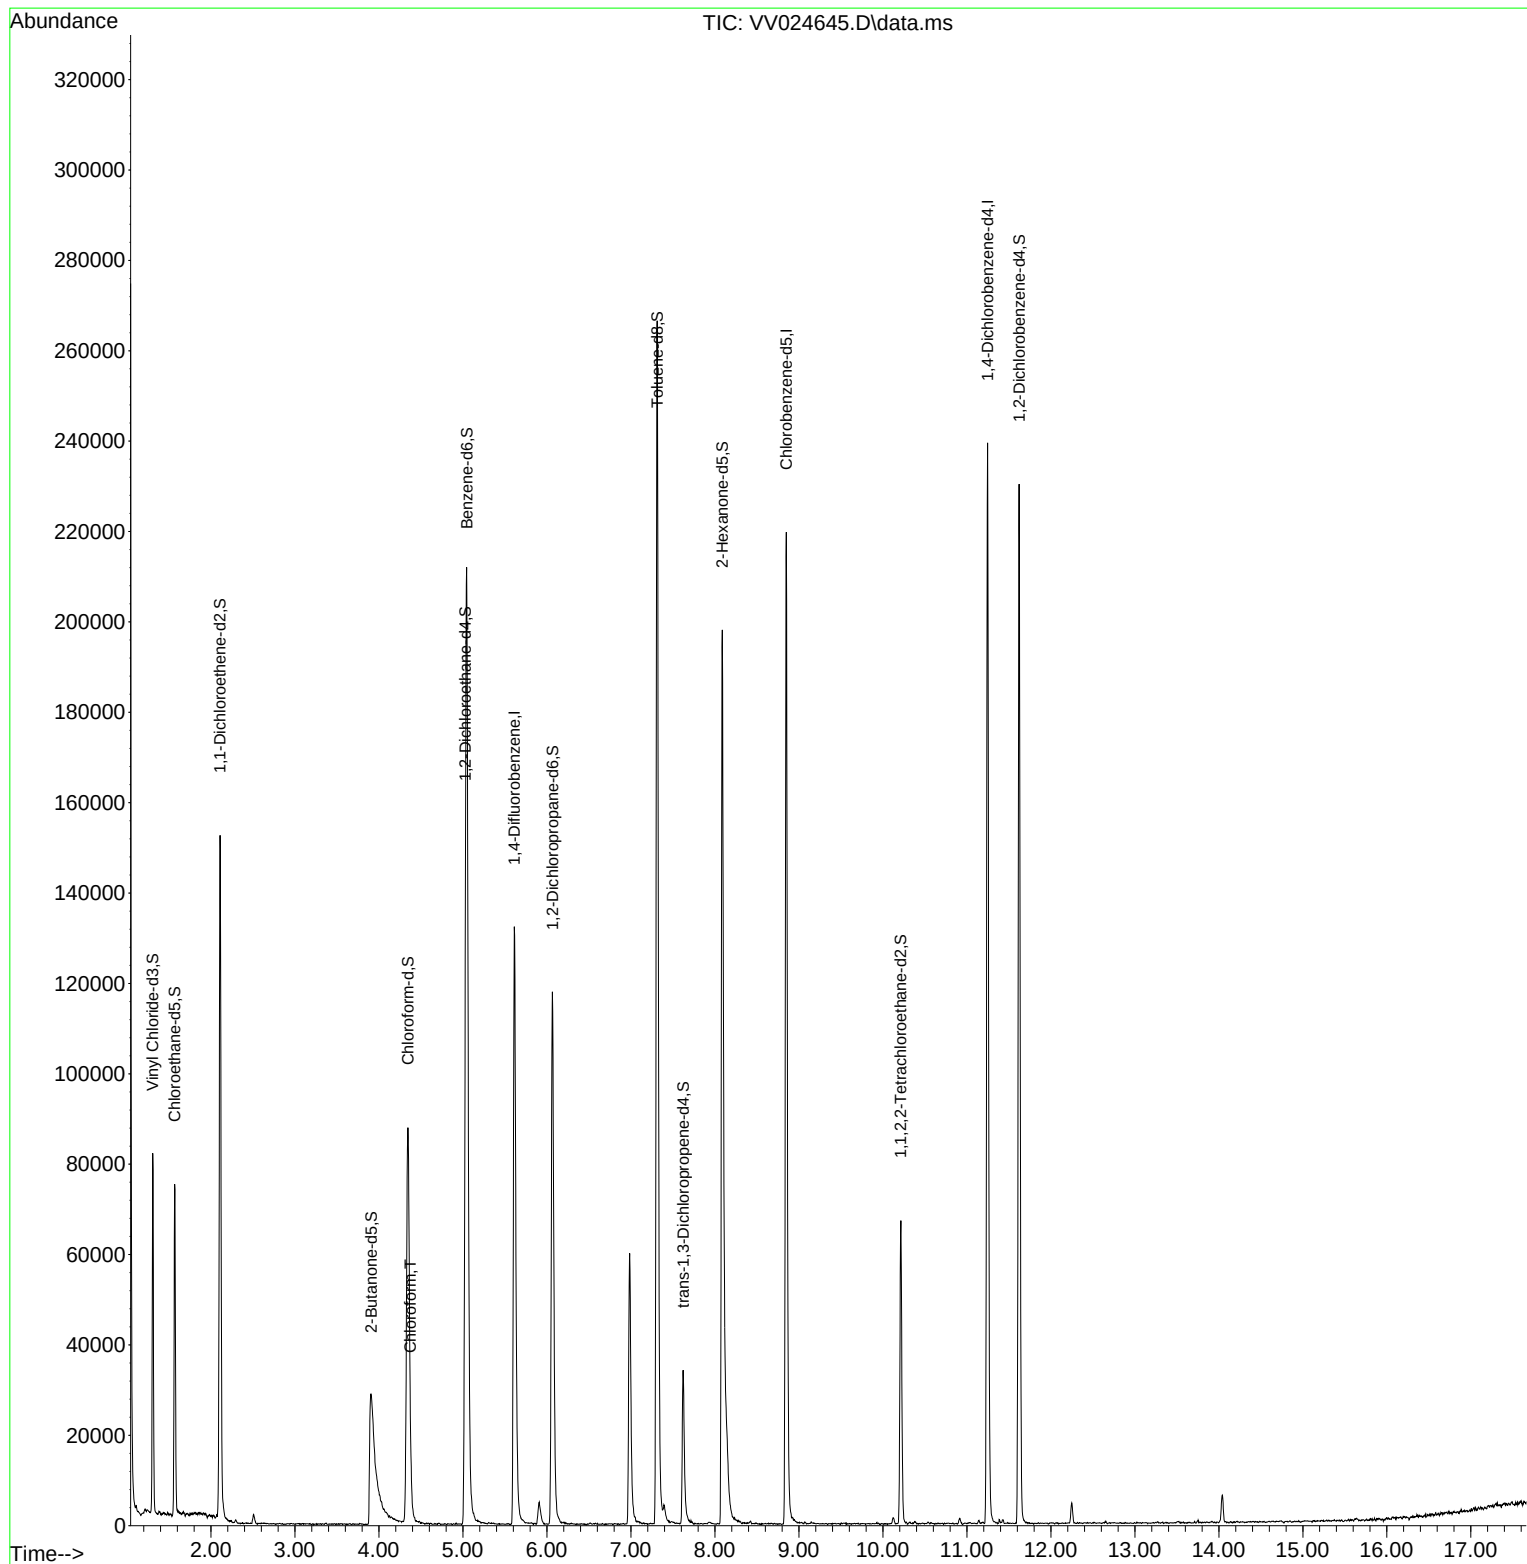

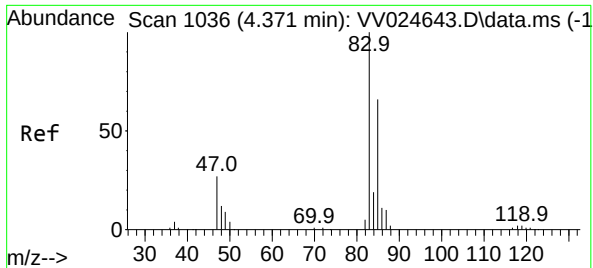

#25

Chloroform

Concen: 0.127 ug/L

RT: 4.375 min Scan# 10

Delta R.T. 0.003 min

Lab File: VV024645.D

Acq: 14 Feb 2022 12:56

Instrument :

MSVOA_V

ClientSampleId :

VHBLK001

Tgt Ion: 83 Resp: 2735

Ion Ratio Lower Upper

83 100

85 85.5 45.2 84.0#

