

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021422\
 Data File : VW024646.D
 Acq On : 14 Feb 2022 13:20
 Operator : SY/MD
 Sample : N1512-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 15 06:27:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 15 06:26:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	112316	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	112876	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56064	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	47697	5.066	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.400%	
7) Chloroethane-d5	1.568	69	43454	5.460	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	109.200%	
11) 1,1-Dichloroethene-d2	2.108	63	78043	3.790	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.800%	
20) 2-Butanone-d5	3.908	46	90433	57.862	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.720%	
24) Chloroform-d	4.349	84	89219	5.384	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.600%	
26) 1,2-Dichloroethane-d4	5.034	65	43302	5.759	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	115.200%	
32) Benzene-d6	5.050	84	183447	5.728	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	114.600%	
36) 1,2-Dichloropropane-d6	6.069	67	55802	5.602	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	112.000%	
41) Toluene-d8	7.317	98	169364	5.670	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.400%	
43) trans-1,3-Dichloroprop...	7.622	79	19971	4.965	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.200%	
46) 2-Hexanone-d5	8.088	63	73908	52.150	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.300%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	31699	5.345	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	51313	5.678	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds					Qvalue	
25) Chloroform	4.378	83	2659	0.129	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024646.D
Acq On : 14 Feb 2022 13:20
Operator : SY/MD
Sample : N1512-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 15 06:27:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

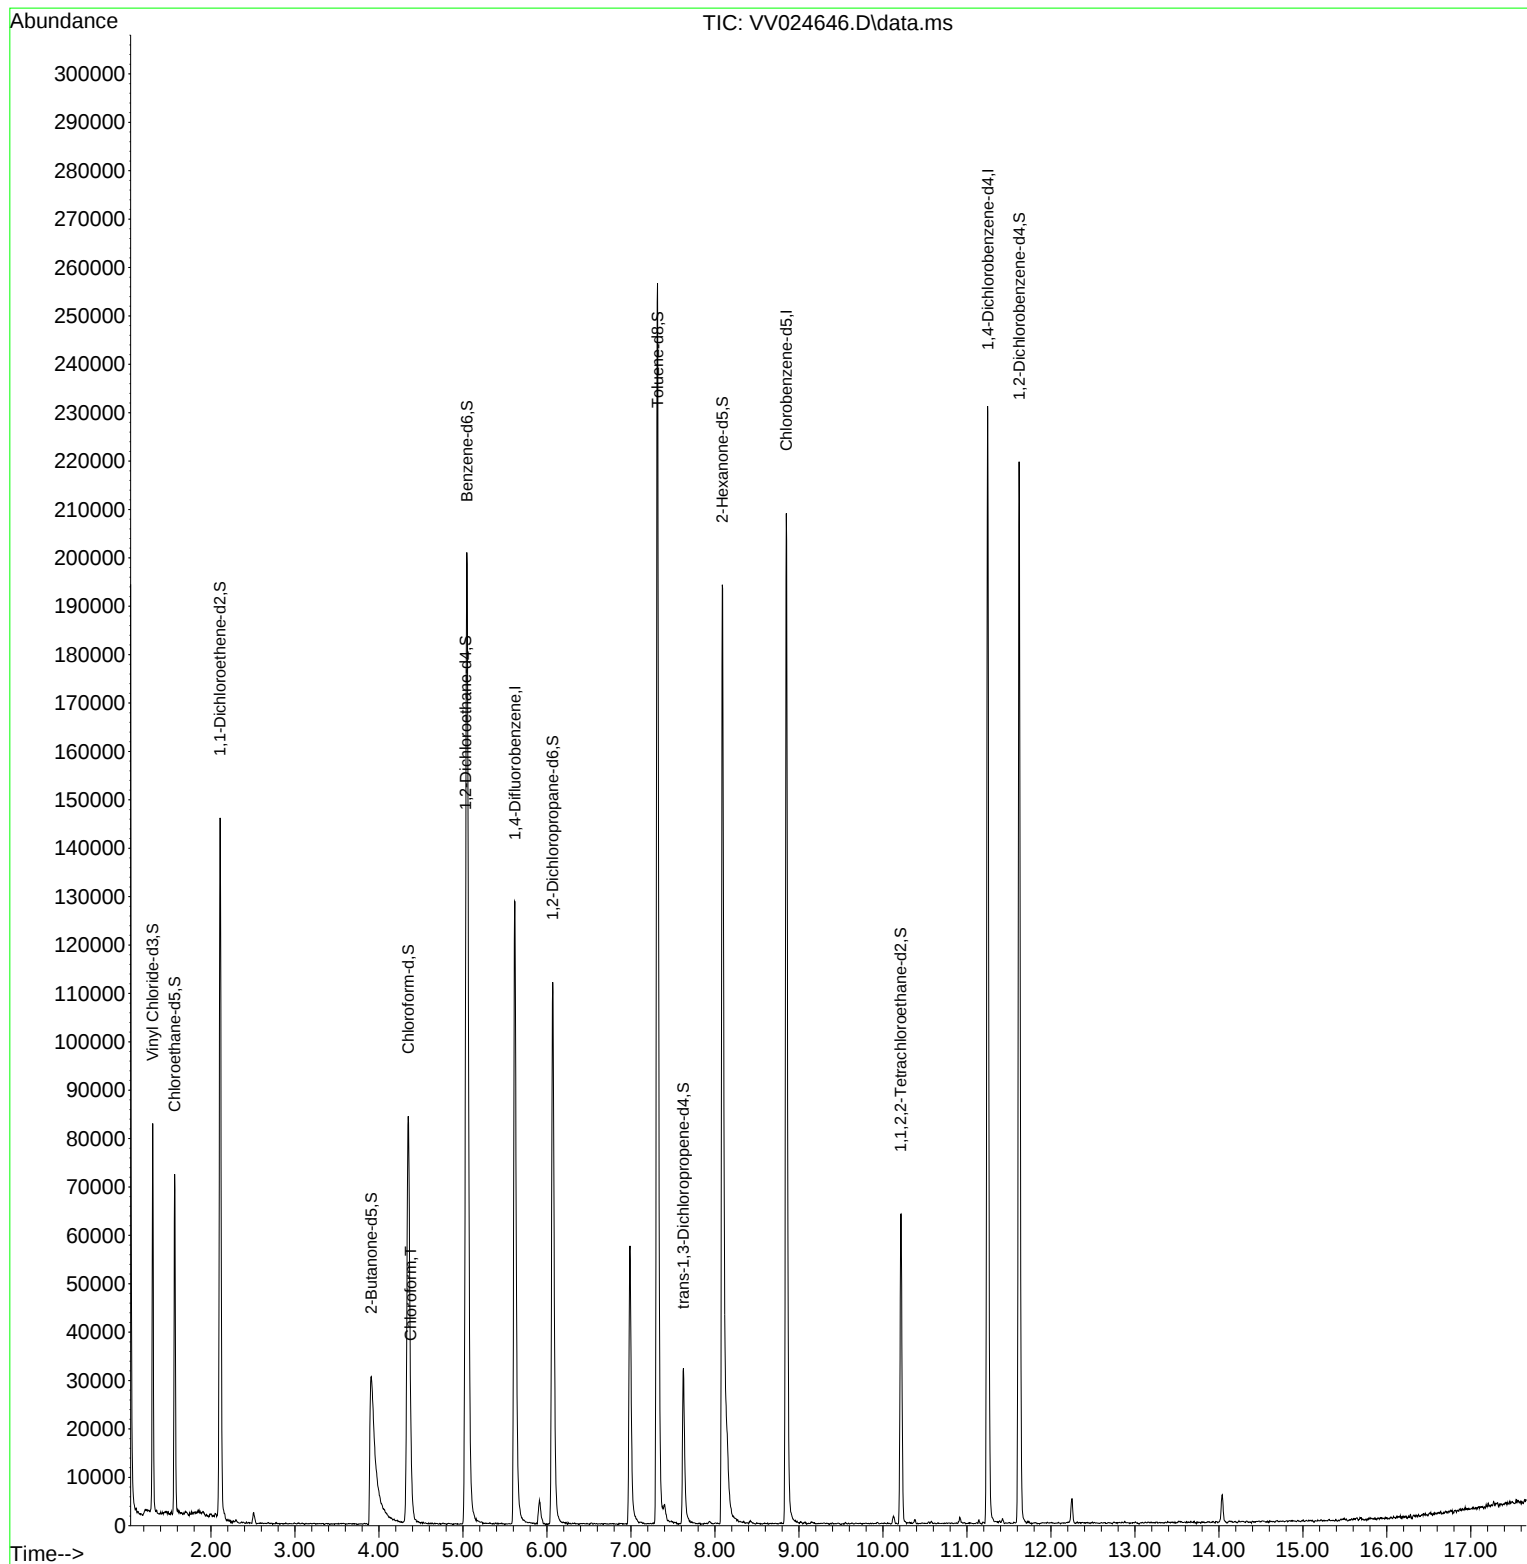

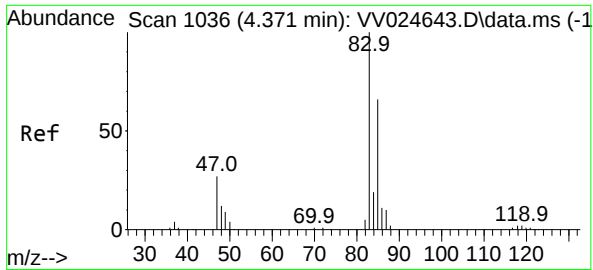

#25
Chloroform
Concen: 0.129 ug/L
RT: 4.378 min Scan# 10
Delta R.T. 0.006 min
Lab File: VV024646.D
Acq: 14 Feb 2022 13:20

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 2659
Ion Ratio Lower Upper
83 100
85 70.4 45.2 84.0

