

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021422\
 Data File : VW024653.D
 Acq On : 14 Feb 2022 16:03
 Operator : SY/MD
 Sample : N1476-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 15 06:28:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 15 06:26:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122858	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	122441	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60827	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	46862	4.550	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.571	69	44965	5.165	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.200%	
11) 1,1-Dichloroethene-d2	2.111	63	76230	3.384	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.895	46	91556	53.554	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.100%	
24) Chloroform-d	4.352	84	91743	5.062	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.034	65	44261	5.382	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.600%	
32) Benzene-d6	5.050	84	189408	5.452	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	109.000%	
36) 1,2-Dichloropropane-d6	6.072	67	56554	5.234	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.600%	
41) Toluene-d8	7.317	98	171187	5.283	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.600%	
43) trans-1,3-Dichloroprop...	7.625	79	20202	4.630	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	92.600%	
46) 2-Hexanone-d5	8.088	63	75815	49.317	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.640%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31726	4.931	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52753	5.380	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.600%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	2831	0.125	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024653.D
Acq On : 14 Feb 2022 16:03
Operator : SY/MD
Sample : N1476-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 15 06:28:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

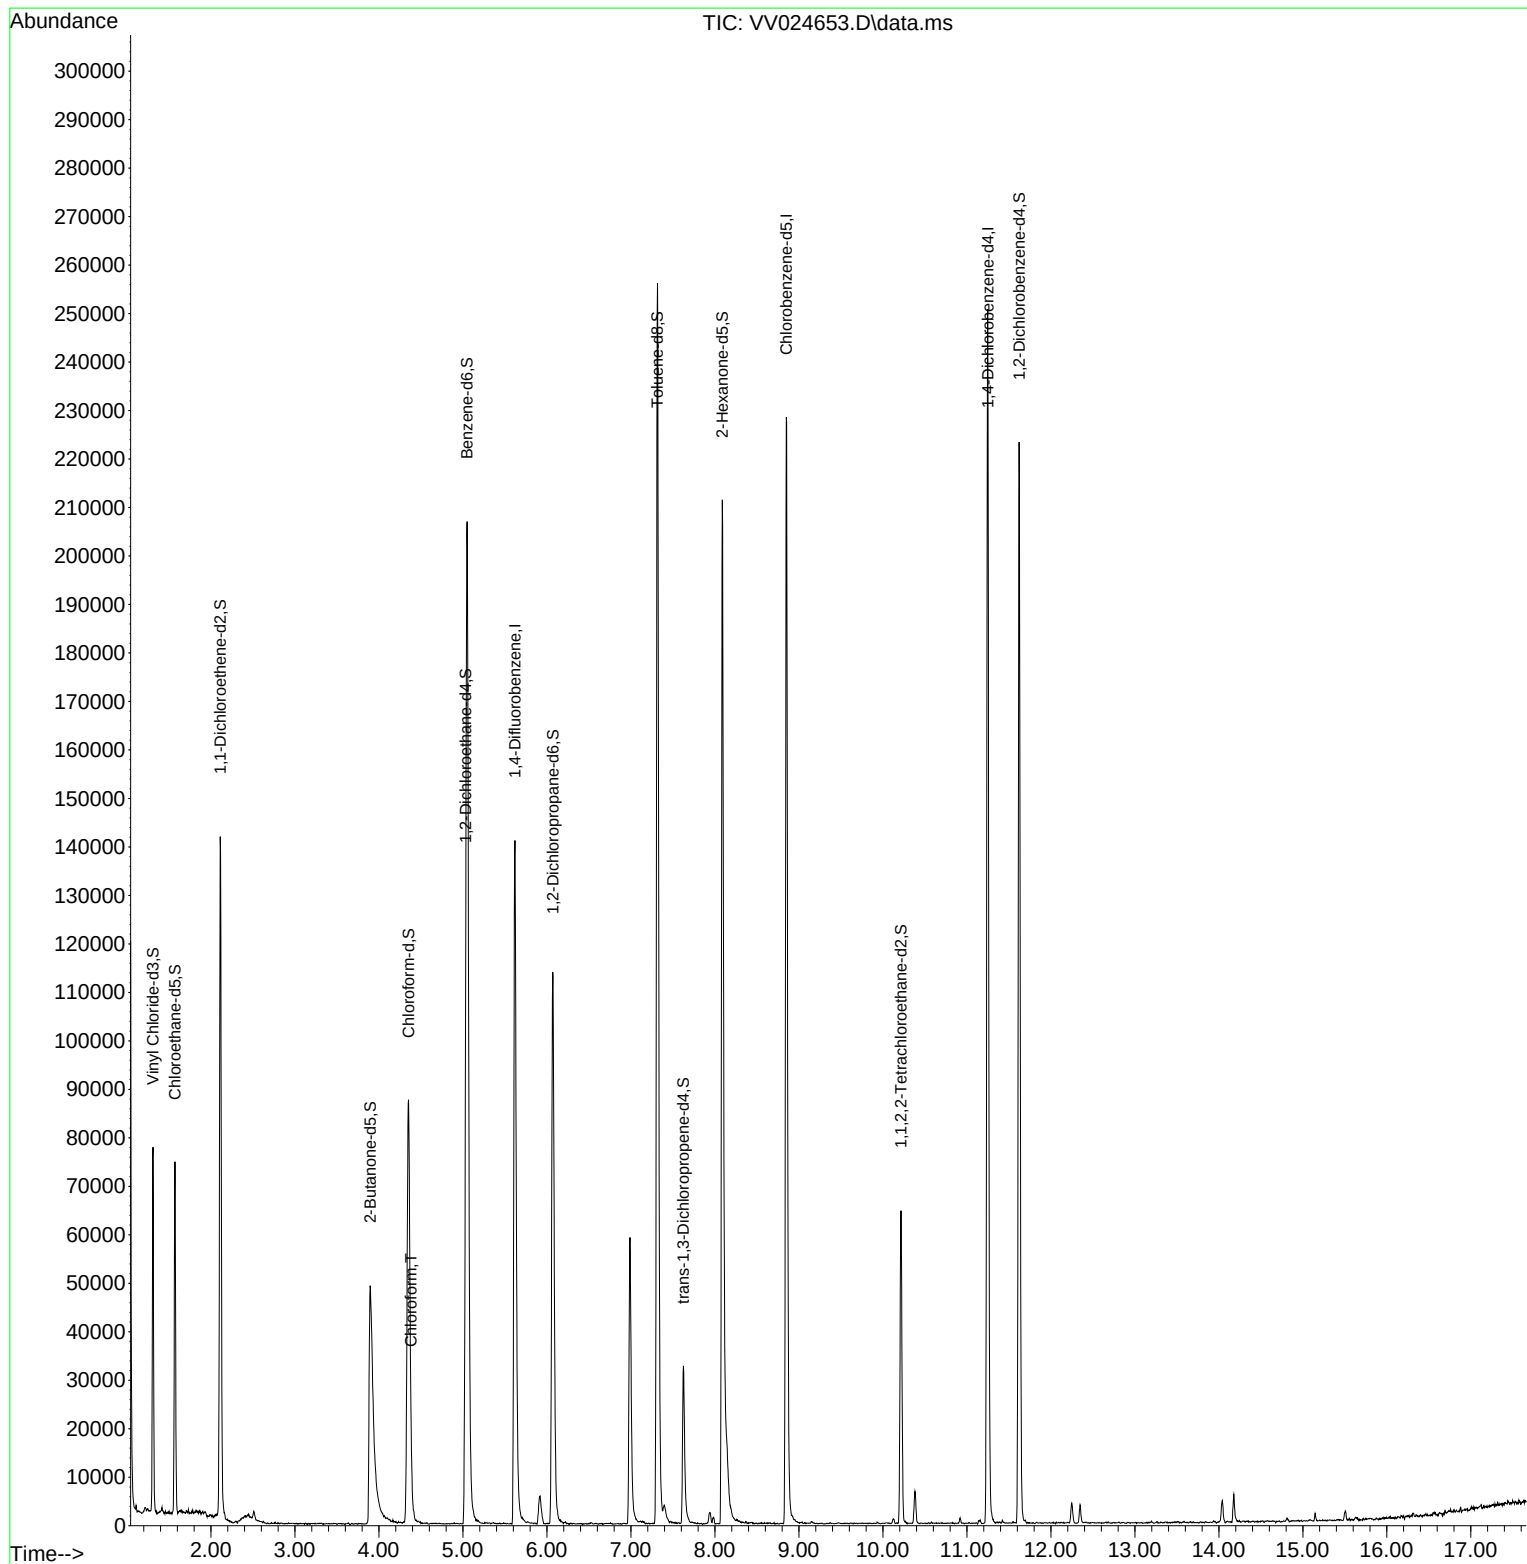

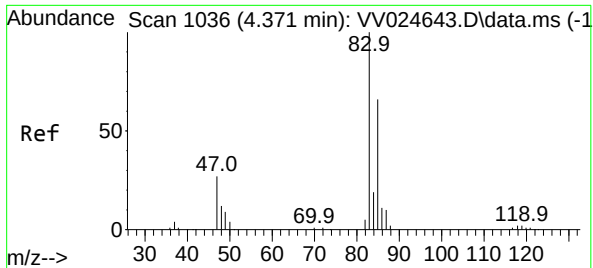

#25
 Chloroform
 Concen: 0.125 ug/L
 RT: 4.381 min Scan# 10
 Delta R.T. 0.010 min
 Lab File: VV024653.D
 Acq: 14 Feb 2022 16:03

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 83 Resp: 2831
 Ion Ratio Lower Upper
 83 100
 85 55.7 45.2 84.0

