

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021422\
 Data File : VW024663.D
 Acq On : 14 Feb 2022 19:56
 Operator : SY/MD
 Sample : N1480-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY5

Quant Time: Feb 15 06:31:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Feb 15 06:26:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	112166	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	112076	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55809	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	43053	4.579	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.600%	
7) Chloroethane-d5	1.571	69	40958	5.153	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2	2.111	63	68917	3.351	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.908	46	85718	54.918	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.840%	
24) Chloroform-d	4.352	84	83826	5.066	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.037	65	40511	5.395	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	108.000%	
32) Benzene-d6	5.053	84	172590	5.427	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	108.600%	
36) 1,2-Dichloropropane-d6	6.069	67	53093	5.368	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.400%	
41) Toluene-d8	7.317	98	153225	5.166	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.400%	
43) trans-1,3-Dichloroprop...	7.625	79	17956	4.496	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.000%	
46) 2-Hexanone-d5	8.088	63	70726	50.261	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.520%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	28675	4.869	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48109	5.348	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.000%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	3677	0.178	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024663.D
Acq On : 14 Feb 2022 19:56
Operator : SY/MD
Sample : N1480-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY5

Quant Time: Feb 15 06:31:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Feb 15 06:26:19 2022
Response via : Initial Calibration

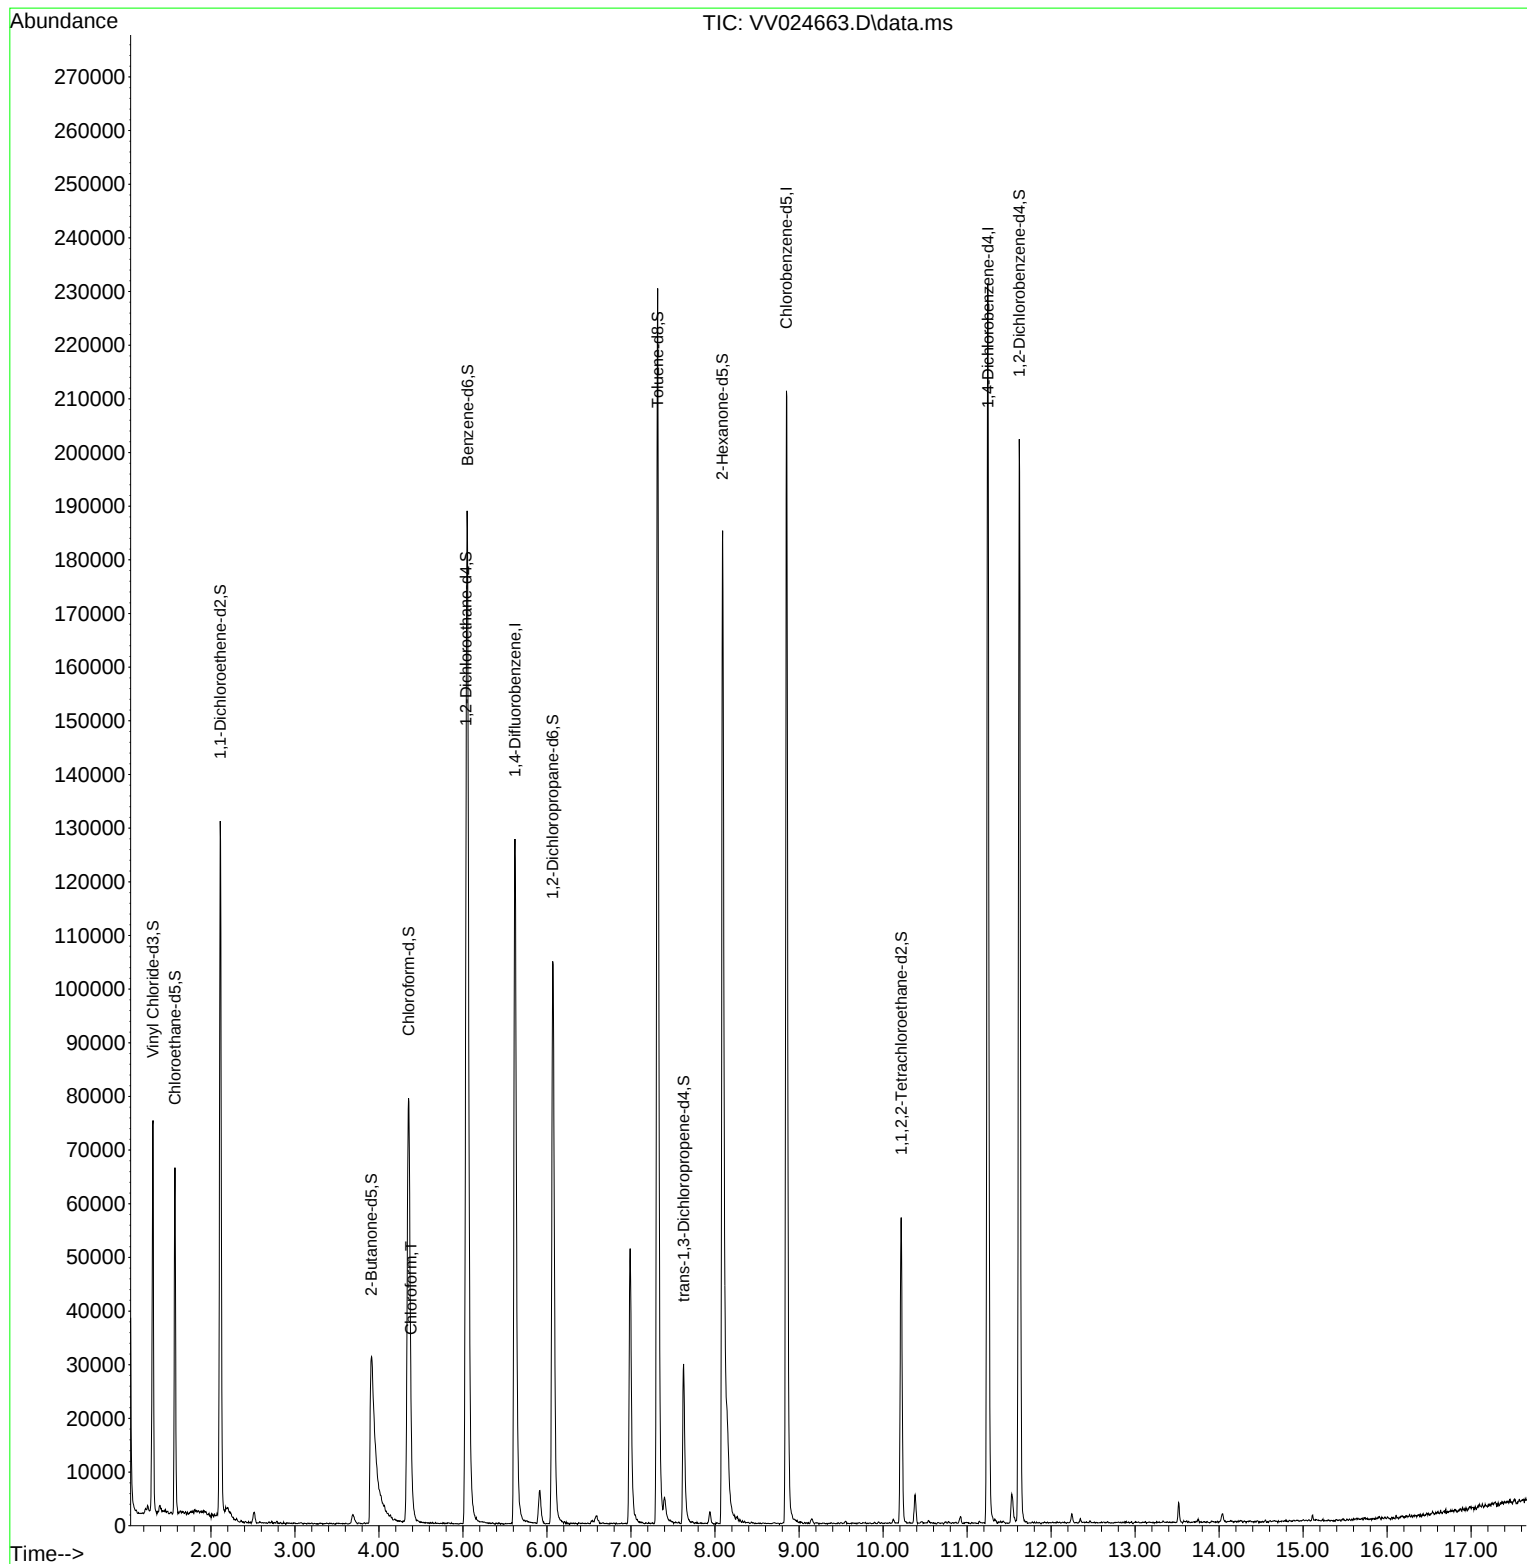

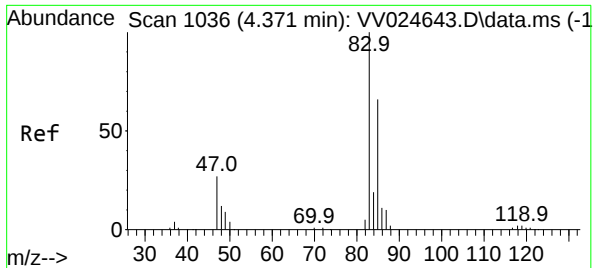

#25

Chloroform

Concen: 0.178 ug/L

RT: 4.381 min Scan# 10

Delta R.T. 0.009 min

Lab File: VV024663.D

Acq: 14 Feb 2022 19:56

Instrument :

MSVOA_V

ClientSampleId :

GBCY5

Tgt Ion: 83 Resp: 3677

Ion Ratio Lower Upper

83 100

85 73.9 45.2 84.0

