

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024644.D
 Acq On : 14 Feb 2022 12:21
 Operator : SY/MD
 Sample : VV0214wBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK304

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	96	rVB	114978	111298	15.31%	1.959%
2	1.571	157	165	178	rBV	99387	112869	15.53%	1.987%
3	2.111	322	333	357	rVB	205537	303402	41.74%	5.340%
4	3.905	879	891	940	rBV2	51019	214702	29.53%	3.779%
5	4.352	1014	1030	1055	rBV	122631	307314	42.27%	5.409%
6	5.050	1229	1247	1276	rBV2	290168	726953	100.00%	12.796%
7	5.616	1412	1423	1445	rBV	180394	369455	50.82%	6.503%
8	5.911	1505	1515	1530	rBV4	6902	14837	2.04%	0.261%
9	6.069	1550	1564	1592	rBV	163980	338507	46.57%	5.958%
10	6.985	1838	1849	1873	rBV	85970	161898	22.27%	2.850%
11	7.317	1939	1952	1972	rBV	371584	652933	89.82%	11.493%
12	7.397	1972	1977	1988	rVB5	4335	8017	1.10%	0.141%
13	7.622	2038	2047	2066	rBV2	47820	86427	11.89%	1.521%
14	8.088	2182	2192	2235	rBV	300675	601438	82.73%	10.586%
15	8.850	2418	2429	2461	rBV	302790	492402	67.74%	8.667%
16	10.214	2837	2853	2871	rBV2	91343	147644	20.31%	2.599%
17	11.246	3163	3174	3193	rBV	332319	506955	69.74%	8.923%
18	11.622	3279	3291	3312	rBV	315452	496017	68.23%	8.731%
19	12.249	3474	3486	3498	rBV	7242	11692	1.61%	0.206%
20	14.040	4028	4043	4056	rBV	9616	16484	2.27%	0.290%




Sum of corrected areas: 5681244

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024644.D
Acq On : 14 Feb 2022 12:21
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

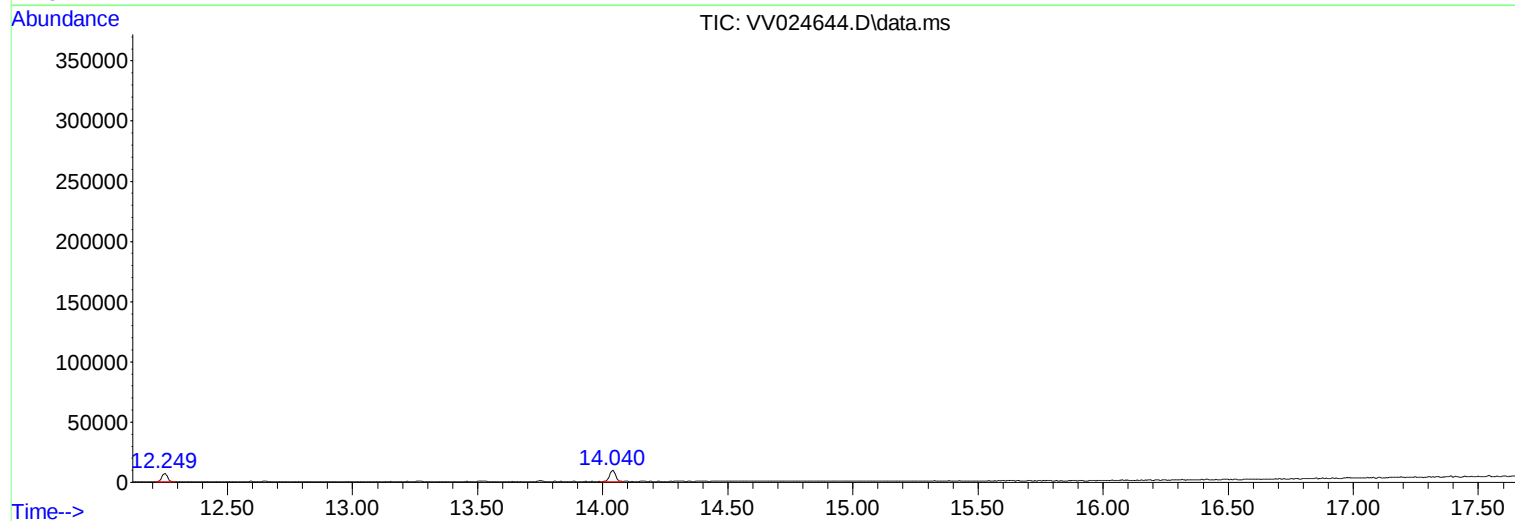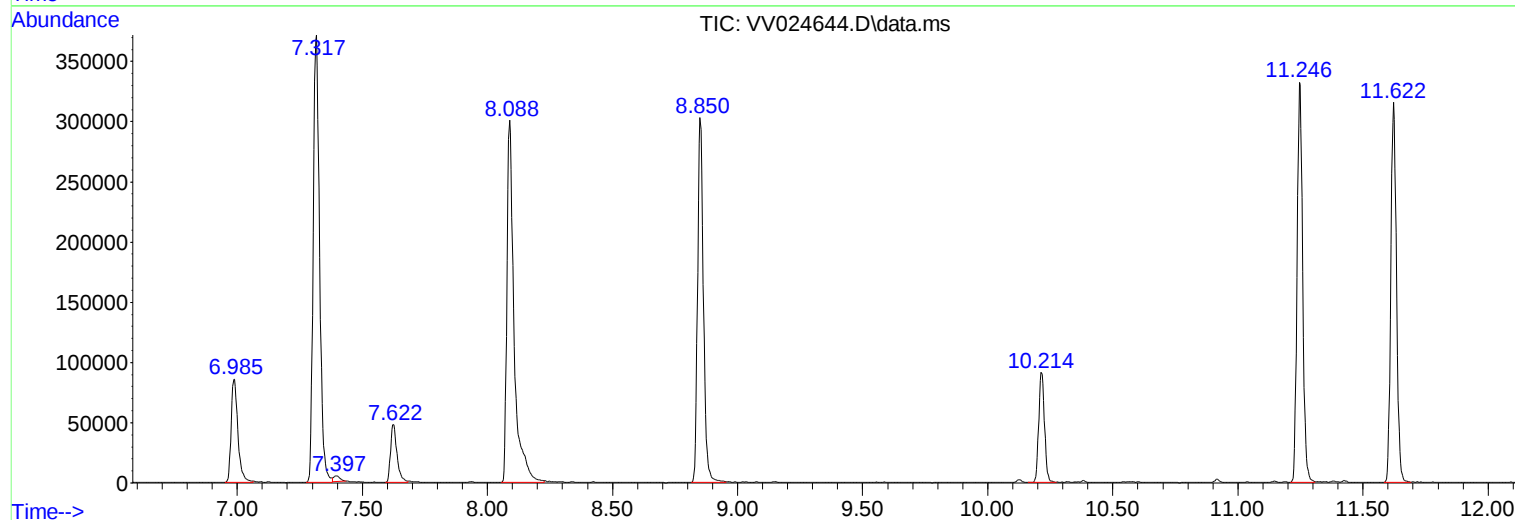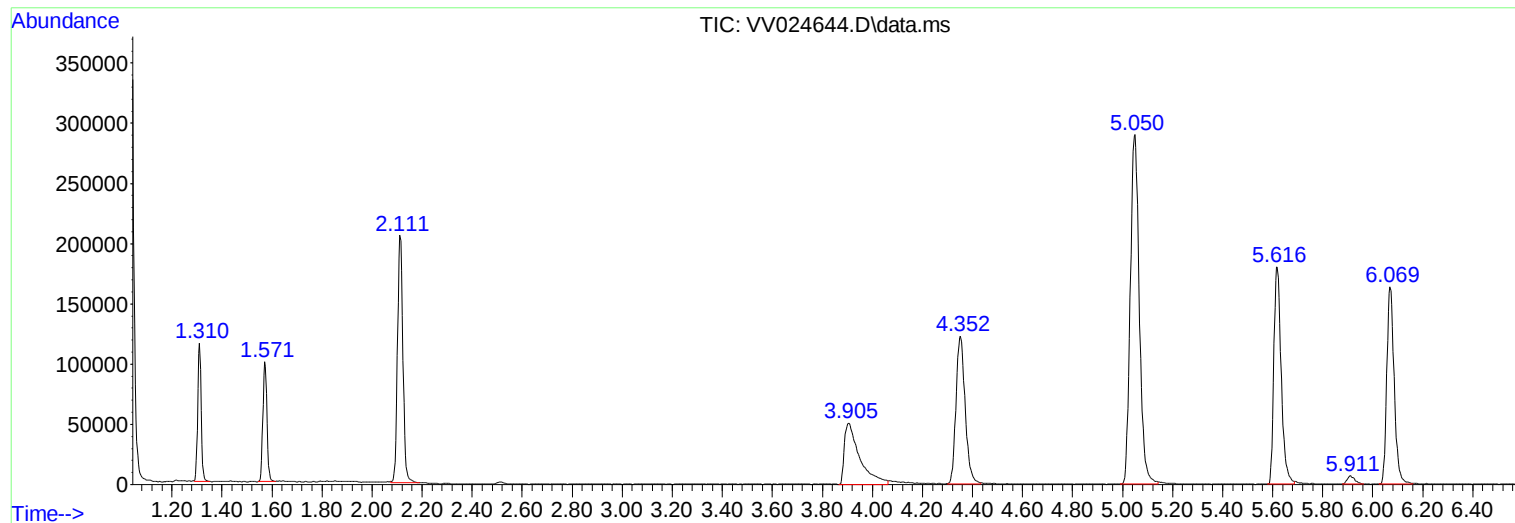

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024644.D
Acq On : 14 Feb 2022 12:21
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected
