

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024645.D
 Acq On : 14 Feb 2022 12:56
 Operator : SY/MD
 Sample : N1479-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	79779	80913	15.36%	1.982%
2	1.568	156	164	175	rBV	73231	83758	15.90%	2.052%
3	2.108	322	332	353	rVB	151120	221938	42.14%	5.436%
4	3.905	875	891	937	rBV2	28921	140897	26.75%	3.451%
5	4.346	1011	1028	1057	rBV	87175	223920	42.52%	5.485%
6	5.043	1226	1245	1280	rBV2	211857	526624	100.00%	12.900%
7	5.612	1411	1422	1451	rBV	132168	270561	51.38%	6.627%
8	5.908	1502	1514	1530	rBV6	4953	11150	2.12%	0.273%
9	6.066	1546	1563	1595	rBV	117855	245342	46.59%	6.010%
10	6.985	1838	1849	1867	rBV	59851	111705	21.21%	2.736%
11	7.313	1939	1951	1971	rBV	266213	467908	88.85%	11.461%
12	7.394	1974	1976	1993	rVB5	3814	5865	1.11%	0.144%
13	7.622	2037	2047	2073	rBV2	33899	61610	11.70%	1.509%
14	8.088	2181	2192	2235	rBV	197836	423079	80.34%	10.363%
15	8.850	2418	2429	2449	rBV	219483	356611	67.72%	8.735%
16	10.214	2842	2853	2871	rBV	67050	104598	19.86%	2.562%
17	11.246	3163	3174	3198	rBV	239121	371988	70.64%	9.112%
18	11.622	3280	3291	3308	rBV	229919	357015	67.79%	8.745%
19	12.249	3477	3486	3494	rBV2	4519	6749	1.28%	0.165%
20	14.040	4030	4043	4053	rBV2	6122	10222	1.94%	0.250%




Sum of corrected areas: 4082453

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024645.D
Acq On : 14 Feb 2022 12:56
Operator : SY/MD
Sample : N1479-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

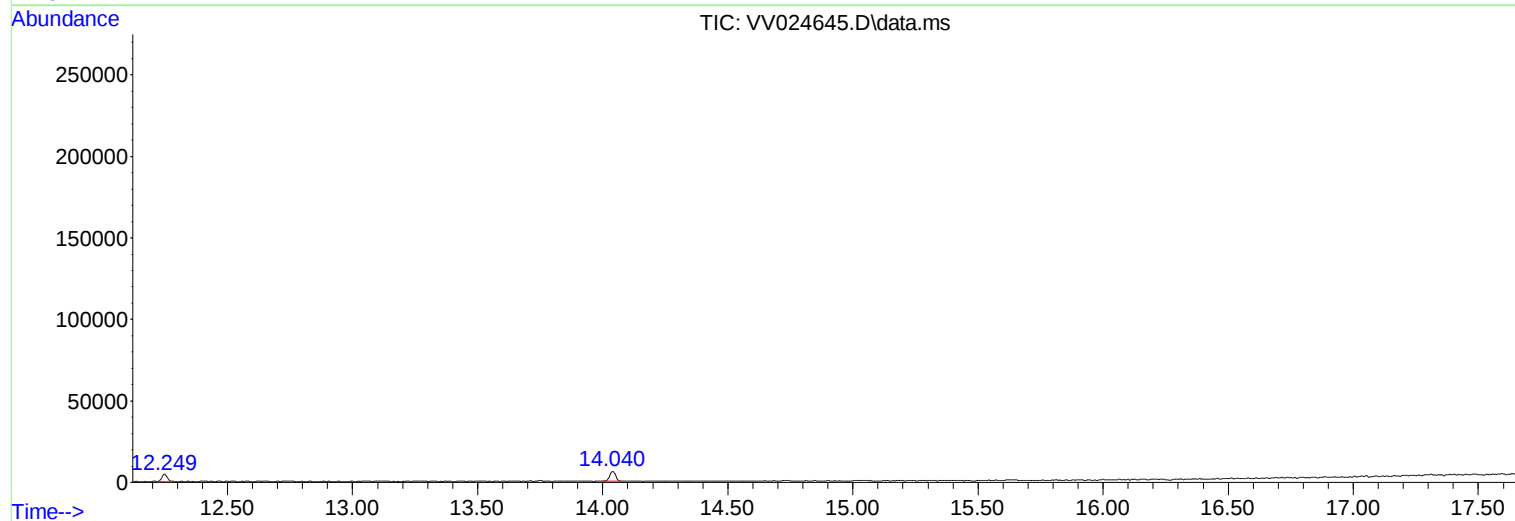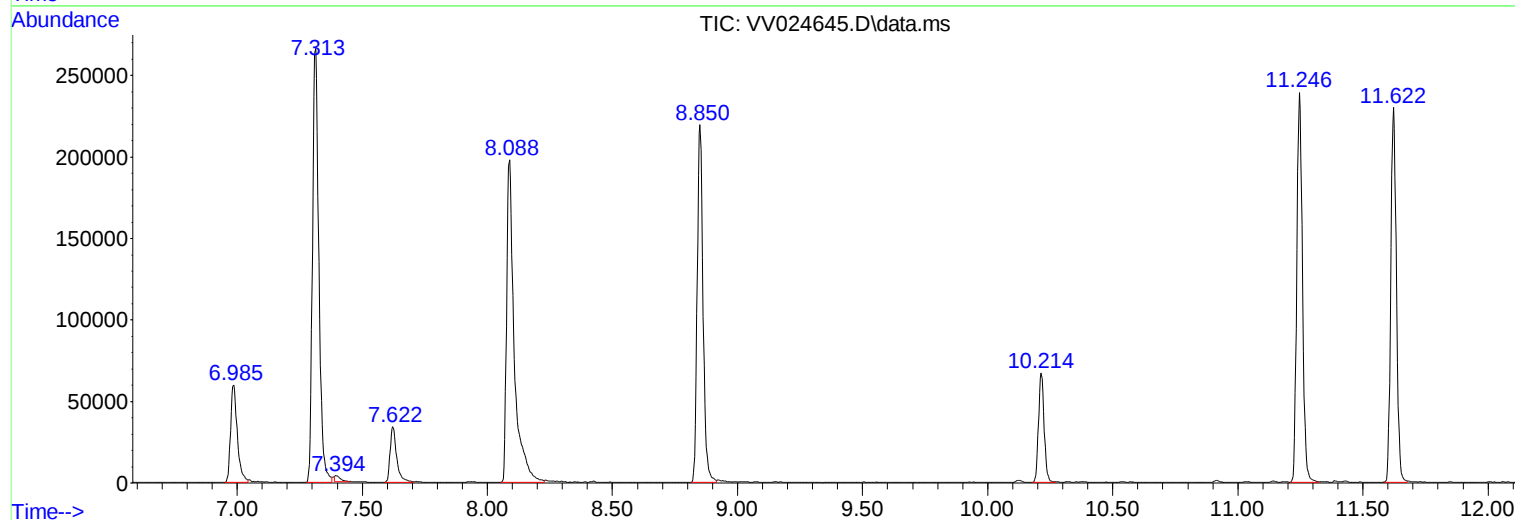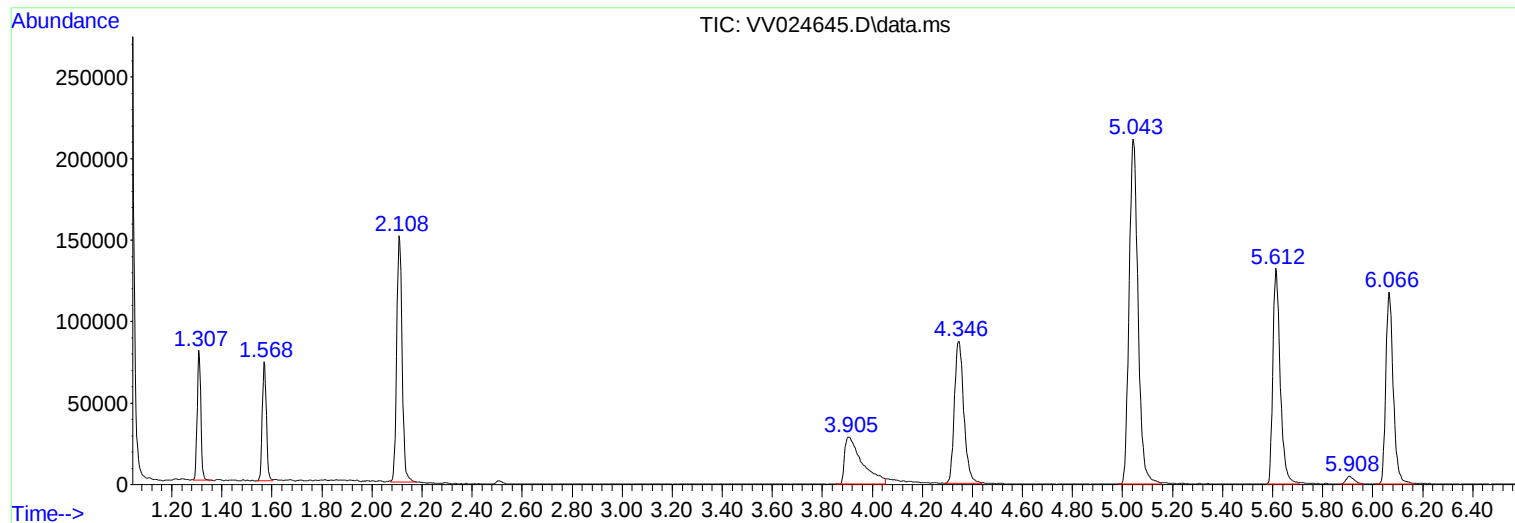

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024645.D
Acq On : 14 Feb 2022 12:56
Operator : SY/MD
Sample : N1479-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024645.D
Acq On : 14 Feb 2022 12:56
Operator : SY/MD
Sample : N1479-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

				---Internal Standard---				
TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
