

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024654.D
 Acq On : 14 Feb 2022 16:26
 Operator : SY/MD
 Sample : N1475-13DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M80DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	98	rVB	75441	81120	7.11%	1.394%
2	1.571	157	165	178	rBV	71528	84844	7.43%	1.458%
3	2.105	320	331	352	rVB	157788	232975	20.41%	4.004%
4	3.902	880	890	934	rBV	42400	166307	14.57%	2.858%
5	4.349	1012	1029	1061	rBV2	94940	250479	21.94%	4.305%
6	5.047	1231	1246	1281	rBV2	227029	554429	48.56%	9.529%
7	5.616	1412	1423	1451	rBV	183472	372452	32.62%	6.401%
8	5.915	1505	1516	1533	rVB8	5888	13414	1.17%	0.231%
9	6.069	1551	1564	1590	rBV	124599	256769	22.49%	4.413%
10	6.986	1839	1849	1877	rBV	62985	118698	10.40%	2.040%
11	7.317	1940	1952	1963	rBV	281651	491715	43.07%	8.451%
12	7.384	1963	1973	2017	rVB	655494	1141652	100.00%	19.622%
13	7.625	2038	2048	2073	rVB2	36184	64581	5.66%	1.110%
14	8.095	2183	2194	2237	rBV	170965	468194	41.01%	8.047%
15	8.850	2417	2429	2455	rBV	298370	491401	43.04%	8.446%
16	9.564	2639	2651	2665	rBV5	5710	13474	1.18%	0.232%
17	10.217	2843	2854	2866	rBV	70278	111874	9.80%	1.923%
18	11.249	3164	3175	3199	rBV	329946	514649	45.08%	8.845%
19	11.622	3280	3291	3315	rBV	240324	389305	34.10%	6.691%




Sum of corrected areas: 5818332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024654.D
Acq On : 14 Feb 2022 16:26
Operator : SY/MD
Sample : N1475-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

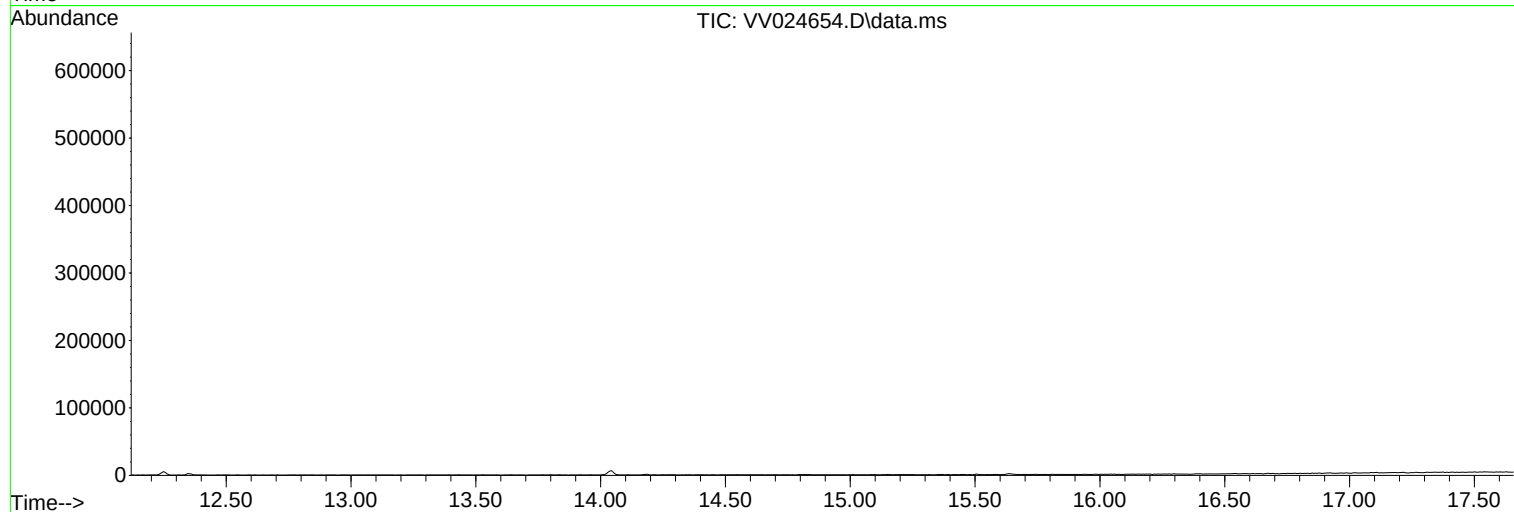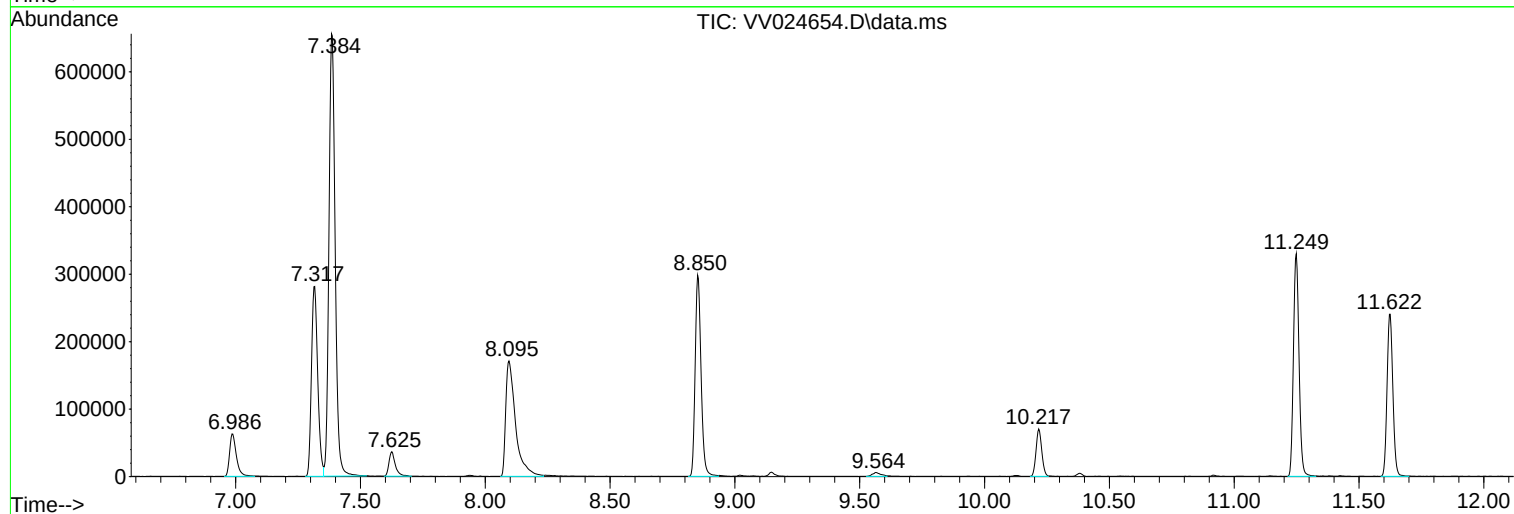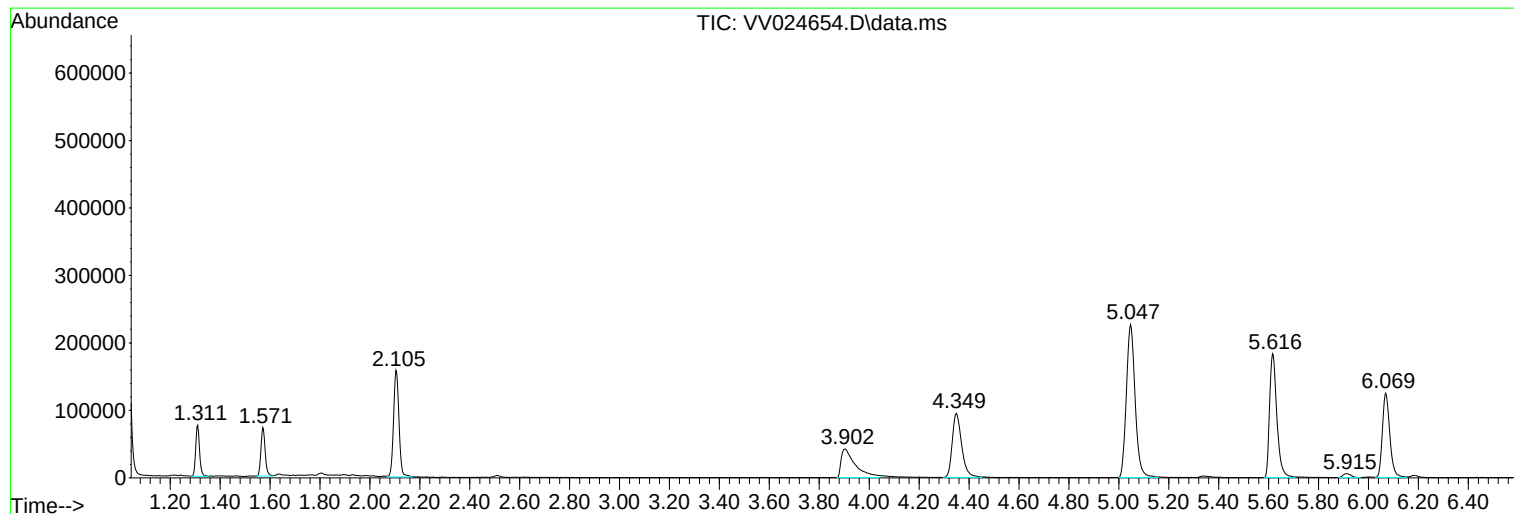

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024654.D
Acq On : 14 Feb 2022 16:26
Operator : SY/MD
Sample : N1475-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024654.D
Acq On : 14 Feb 2022 16:26
Operator : SY/MD
Sample : N1475-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------