

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024655.D
 Acq On : 14 Feb 2022 16:49
 Operator : SY/MD
 Sample : N1475-14DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M81DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	98	rVB	86974	87918	8.23%	1.539%
2	1.571	156	165	176	rBV	83281	94241	8.83%	1.650%
3	2.111	322	333	357	rVB	160084	235732	22.08%	4.126%
4	3.899	879	889	926	rBV	49931	181669	17.01%	3.180%
5	4.349	1013	1029	1056	rBV	102996	264002	24.72%	4.621%
6	5.050	1229	1247	1277	rBV2	239347	599826	56.17%	10.500%
7	5.619	1412	1424	1451	rBV	146293	298170	27.92%	5.219%
8	5.911	1505	1515	1537	rVB4	7037	14673	1.37%	0.257%
9	6.069	1552	1564	1591	rBV	138945	284744	26.67%	4.984%
10	6.989	1838	1850	1875	rBV	70492	131158	12.28%	2.296%
11	7.317	1940	1952	1964	rBV	299554	516109	48.33%	9.034%
12	7.387	1964	1974	2001	rVB	617888	1067786	100.00%	18.691%
13	7.625	2038	2048	2070	rBV	39629	70460	6.60%	1.233%
14	8.088	2181	2192	2244	rBV	263623	521150	48.81%	9.122%
15	8.850	2418	2429	2450	rBV	240573	393936	36.89%	6.896%
16	10.214	2840	2853	2872	rBV	80054	125548	11.76%	2.198%
17	11.246	3163	3174	3195	rBV	266679	409337	38.34%	7.165%
18	11.622	3280	3291	3311	rBV	257025	404869	37.92%	7.087%
19	14.040	4034	4043	4054	rVB2	6957	11521	1.08%	0.202%




Sum of corrected areas: 5712849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024655.D
Acq On : 14 Feb 2022 16:49
Operator : SY/MD
Sample : N1475-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

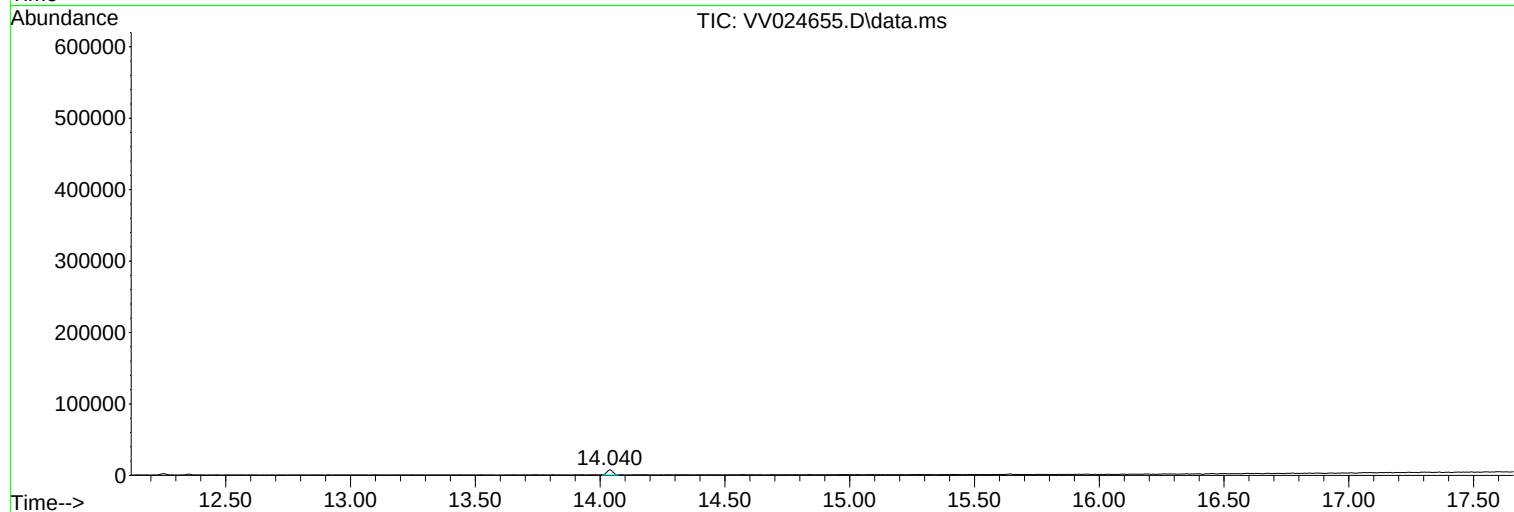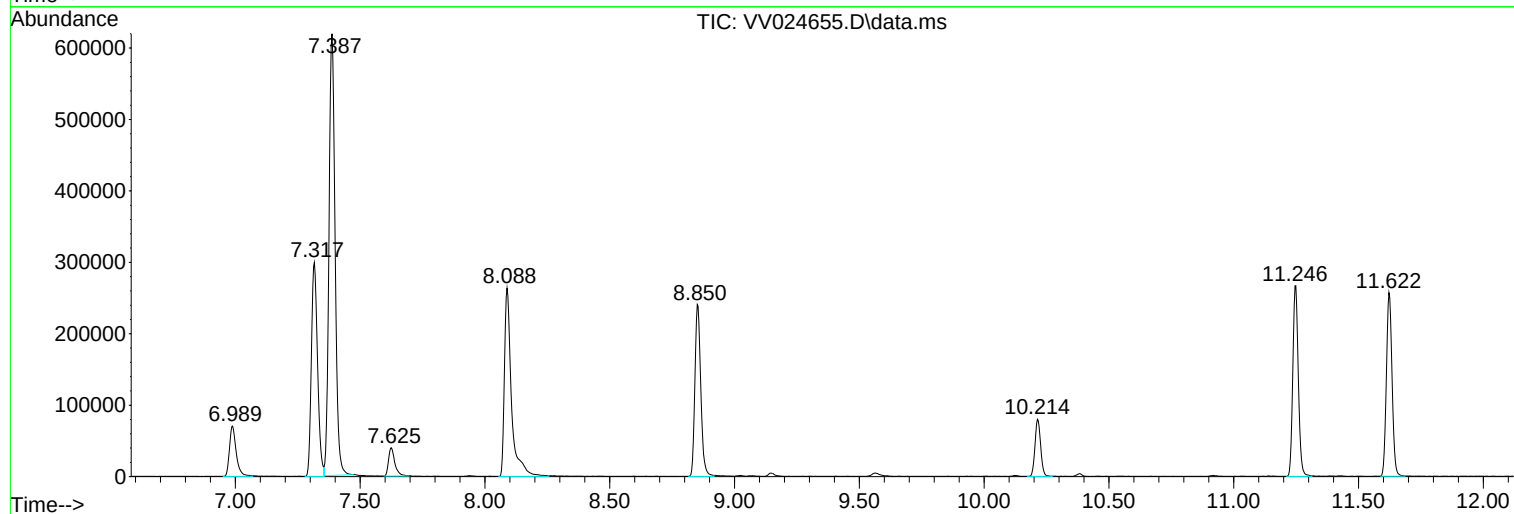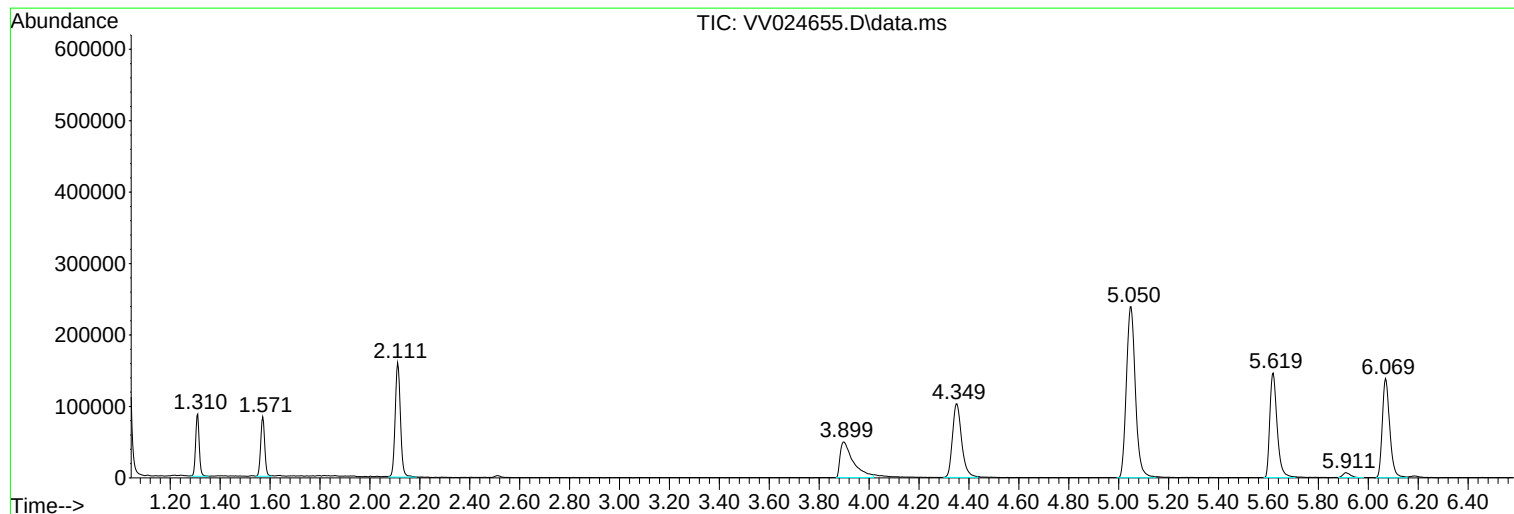

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024655.D
Acq On : 14 Feb 2022 16:49
Operator : SY/MD
Sample : N1475-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024655.D
Acq On : 14 Feb 2022 16:49
Operator : SY/MD
Sample : N1475-14DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M81DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc