

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024656.D
 Acq On : 14 Feb 2022 17:13
 Operator : SY/MD
 Sample : N1475-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	93	rVB	73763	74550	15.23%	1.865%
2	1.571	157	165	180	rVB	68098	76407	15.61%	1.911%
3	2.111	322	333	353	rBV	135950	197032	40.26%	4.929%
4	3.902	880	890	937	rBV	36630	146954	30.03%	3.676%
5	4.352	1013	1030	1060	rBV2	82814	208402	42.59%	5.213%
6	5.050	1230	1247	1275	rBV2	194742	489360	100.00%	12.242%
7	5.619	1411	1424	1451	rBV	144602	296112	60.51%	7.407%
8	5.915	1506	1516	1531	rBV9	5312	12865	2.63%	0.322%
9	6.069	1549	1564	1592	rBV	111086	231819	47.37%	5.799%
10	6.989	1840	1850	1874	rBV	56283	106084	21.68%	2.654%
11	7.317	1940	1952	1971	rBV	245361	431920	88.26%	10.805%
12	7.394	1971	1976	1996	rVB2	5833	12599	2.57%	0.315%
13	7.625	2038	2048	2070	rBV	31679	58380	11.93%	1.460%
14	7.979	2150	2158	2168	rVB4	7393	12233	2.50%	0.306%
15	8.088	2183	2192	2230	rBV	201570	403972	82.55%	10.106%
16	8.850	2418	2429	2453	rBV	235337	386396	78.96%	9.666%
17	10.217	2843	2854	2867	rBV	63426	100169	20.47%	2.506%
18	11.249	3163	3175	3195	rBV	253528	400899	81.92%	10.029%
19	11.622	3279	3291	3313	rBV	217408	342223	69.93%	8.561%
20	14.040	4031	4043	4051	rBV2	6005	9119	1.86%	0.228%




Sum of corrected areas: 3997495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024656.D
Acq On : 14 Feb 2022 17:13
Operator : SY/MD
Sample : N1475-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

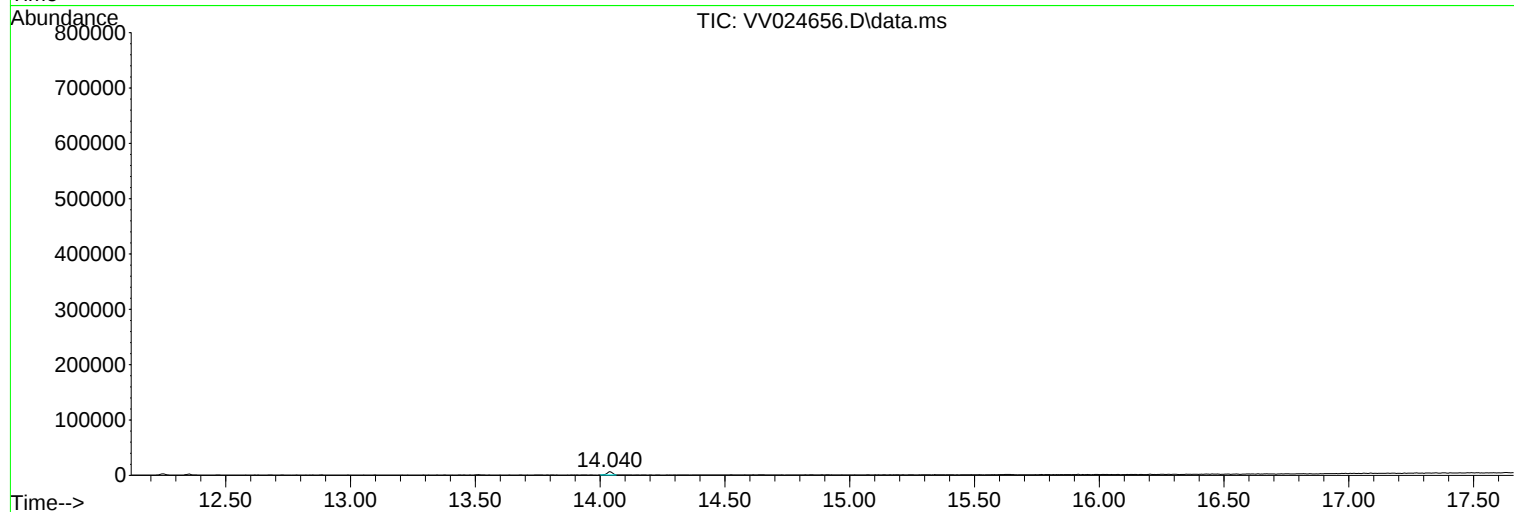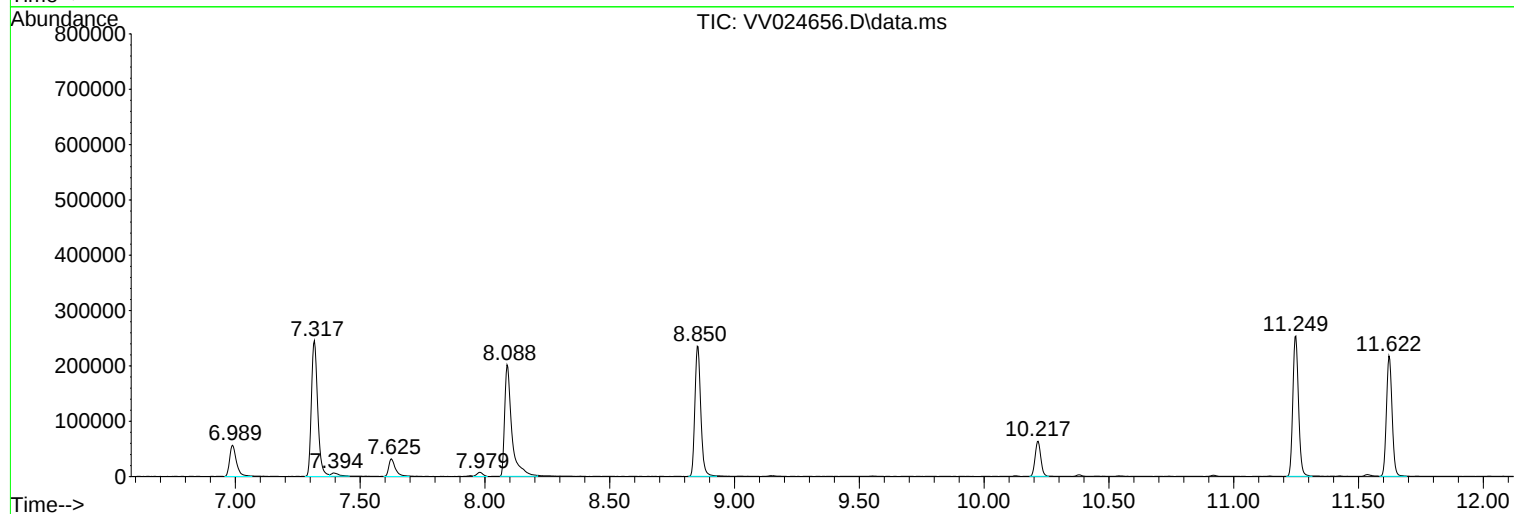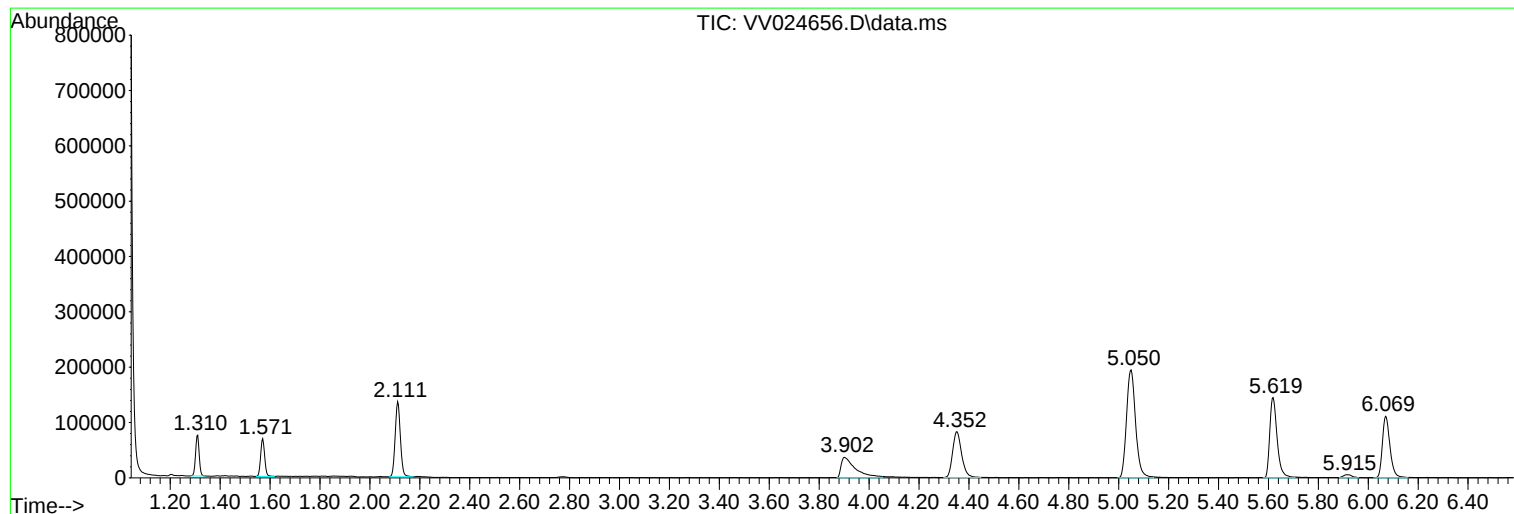

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024656.D
Acq On : 14 Feb 2022 17:13
Operator : SY/MD
Sample : N1475-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024656.D
Acq On : 14 Feb 2022 17:13
Operator : SY/MD
Sample : N1475-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc