

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024662.D
 Acq On : 14 Feb 2022 19:32
 Operator : SY/MD
 Sample : N1480-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	74	84	98	rVB	74653	87838	18.20%	2.279%
2	1.571	157	165	177	rBV	67168	76476	15.84%	1.984%
3	2.111	322	333	348	rVV	131798	191698	39.71%	4.974%
4	2.201	348	361	378	rVB5	1991	6097	1.26%	0.158%
5	3.902	879	890	931	rBV	36963	145557	30.15%	3.777%
6	4.352	1012	1030	1063	rBV	81697	212390	44.00%	5.511%
7	5.050	1232	1247	1279	rBV2	193810	482713	100.00%	12.526%
8	5.619	1413	1424	1456	rBV	131303	265645	55.03%	6.893%
9	5.908	1505	1514	1530	rBV4	6304	13263	2.75%	0.344%
10	6.072	1551	1565	1587	rBV	109851	226857	47.00%	5.887%
11	6.989	1840	1850	1872	rBV2	54689	102783	21.29%	2.667%
12	7.317	1941	1952	1971	rBV	239841	418319	86.66%	10.855%
13	7.397	1973	1977	1993	rVB3	4761	8263	1.71%	0.214%
14	7.625	2039	2048	2071	rBV	30120	55855	11.57%	1.449%
15	8.088	2182	2192	2230	rBV	195696	401815	83.24%	10.427%
16	8.850	2418	2429	2458	rBV	211875	348966	72.29%	9.055%
17	10.214	2843	2853	2870	rBV	60270	94692	19.62%	2.457%
18	10.381	2896	2905	2919	rVB4	4562	7510	1.56%	0.195%
19	11.246	3164	3174	3199	rBV	231101	362081	75.01%	9.395%
20	11.535	3256	3264	3276	rBV3	4237	8085	1.67%	0.210%
21	11.622	3280	3291	3313	rVB	210568	331116	68.59%	8.592%
22	14.037	4032	4042	4054	rBV2	3528	5752	1.19%	0.149%




Sum of corrected areas: 3853771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024662.D
Acq On : 14 Feb 2022 19:32
Operator : SY/MD
Sample : N1480-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

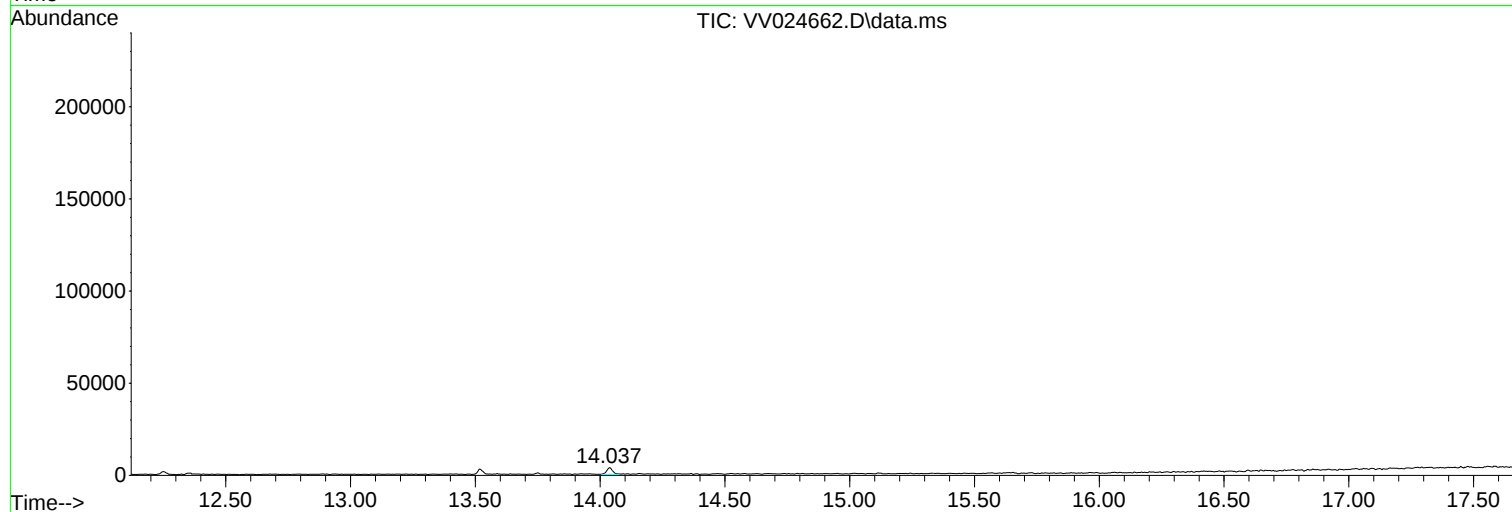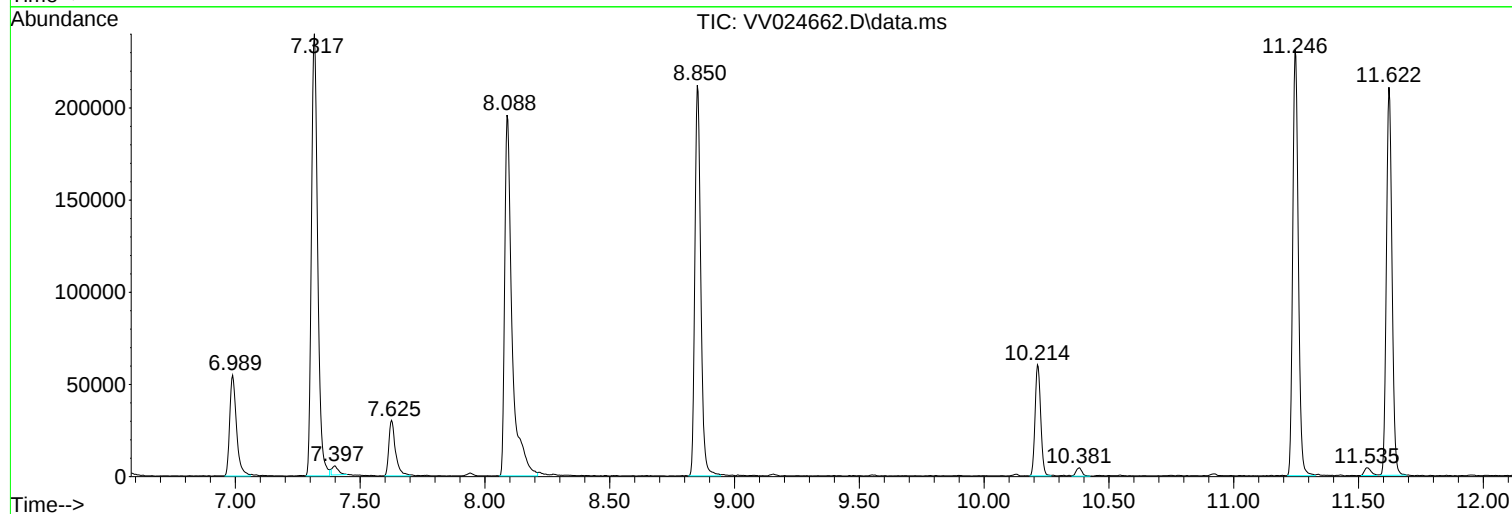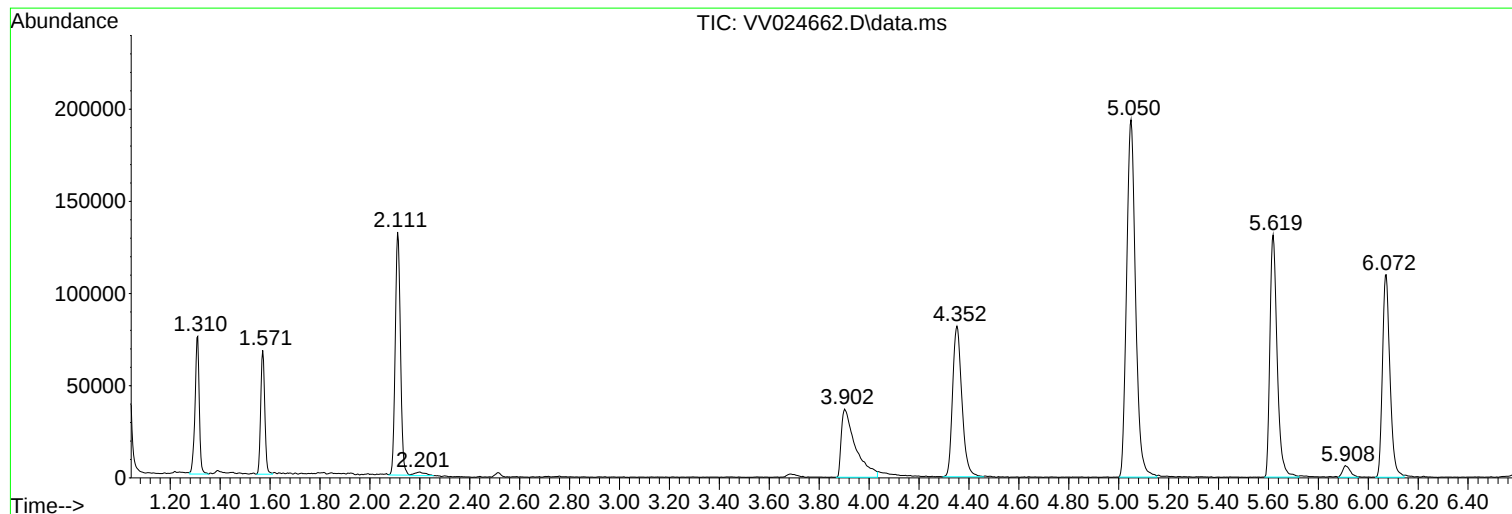

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024662.D
Acq On : 14 Feb 2022 19:32
Operator : SY/MD
Sample : N1480-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024662.D
Acq On : 14 Feb 2022 19:32
Operator : SY/MD
Sample : N1480-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc