

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024663.D
 Acq On : 14 Feb 2022 19:56
 Operator : SY/MD
 Sample : N1480-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	73	84	96	rVB2	73013	86659	18.48%	2.319%
2	1.571	157	165	176	rBV	64510	73392	15.65%	1.964%
3	2.111	323	333	347	rBV	129301	186439	39.76%	4.988%
4	3.912	880	893	926	rBV2	31054	129415	27.60%	3.462%
5	4.352	1013	1030	1059	rBV2	78885	204720	43.65%	5.477%
6	5.050	1231	1247	1279	rBV2	188773	468961	100.00%	12.547%
7	5.619	1413	1424	1457	rBV	127530	260781	55.61%	6.977%
8	5.915	1505	1516	1529	rBV5	6157	12794	2.73%	0.342%
9	6.069	1550	1564	1593	rBV	104804	221006	47.13%	5.913%
10	6.989	1838	1850	1874	rBV2	51298	99468	21.21%	2.661%
11	7.317	1937	1952	1971	rBV	230237	403919	86.13%	10.807%
12	7.400	1972	1978	1995	rVB4	4477	9357	2.00%	0.250%
13	7.625	2038	2048	2067	rBV	29766	53692	11.45%	1.437%
14	8.091	2183	2193	2236	rBV	185028	393898	83.99%	10.539%
15	8.850	2419	2429	2455	rBV	210930	346310	73.85%	9.266%
16	10.217	2843	2854	2869	rBV	56985	90344	19.26%	2.417%
17	10.381	2896	2905	2914	rVB2	5397	8220	1.75%	0.220%
18	11.246	3164	3174	3197	rBV	231086	358887	76.53%	9.602%
19	11.532	3253	3263	3272	rBV3	5445	9714	2.07%	0.260%
20	11.622	3280	3291	3313	rVB	201797	319643	68.16%	8.552%




Sum of corrected areas: 3737619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024663.D
Acq On : 14 Feb 2022 19:56
Operator : SY/MD
Sample : N1480-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

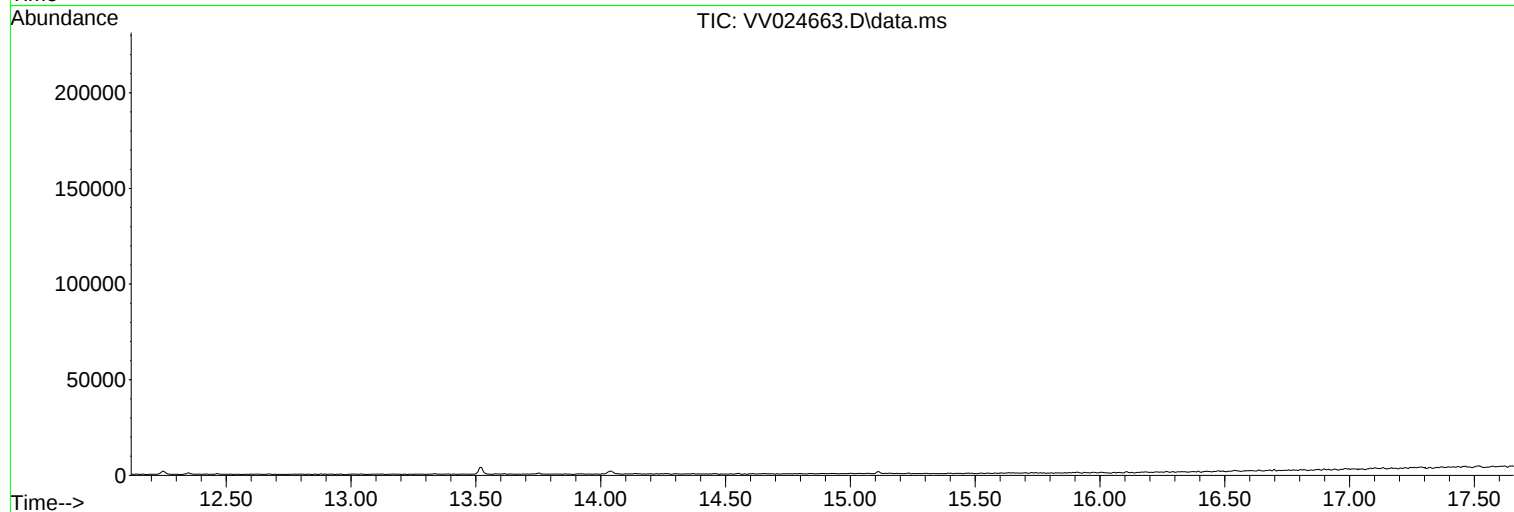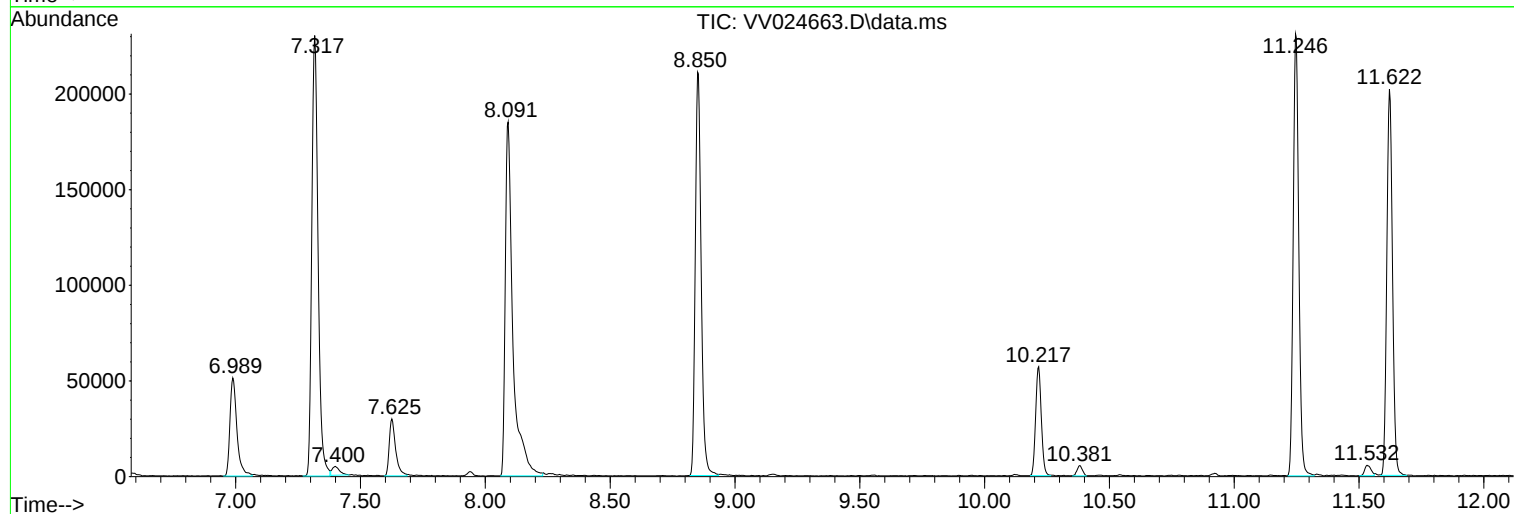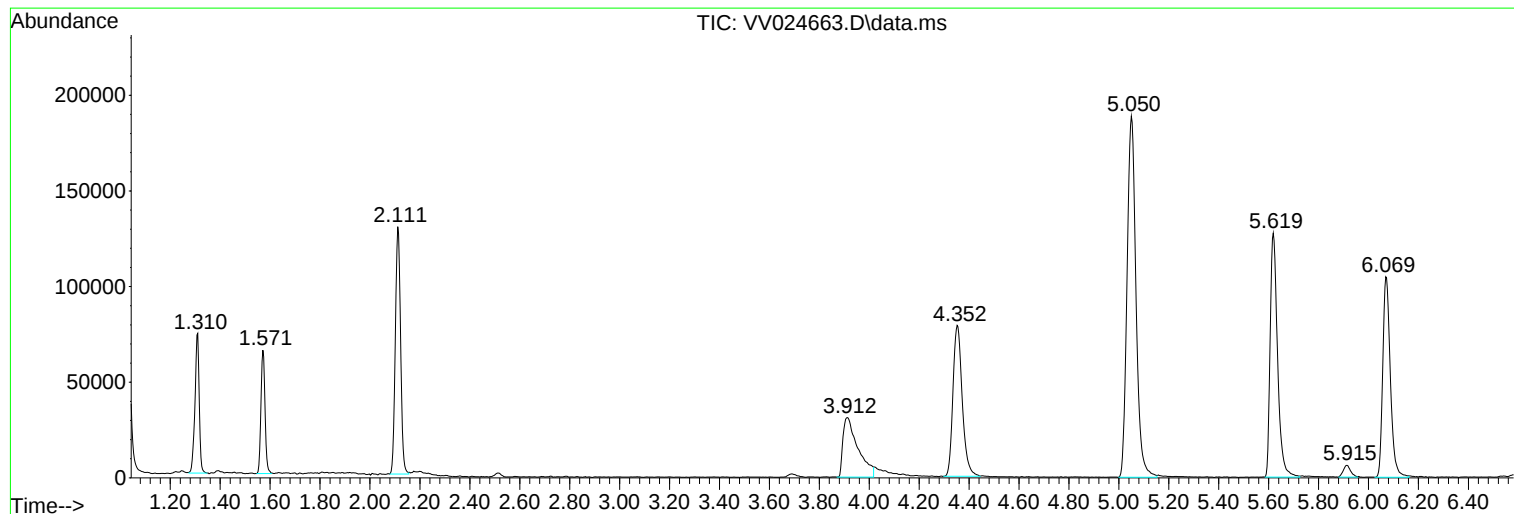

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024663.D
Acq On : 14 Feb 2022 19:56
Operator : SY/MD
Sample : N1480-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
Data File : VV024663.D
Acq On : 14 Feb 2022 19:56
Operator : SY/MD
Sample : N1480-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc