


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021422\
 Data File : VV024642.D
 Acq On : 14 Feb 2022 09:00
 Operator : SY/MD
 Sample : BFB269
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB269

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Feb 16 23:36:08 2022

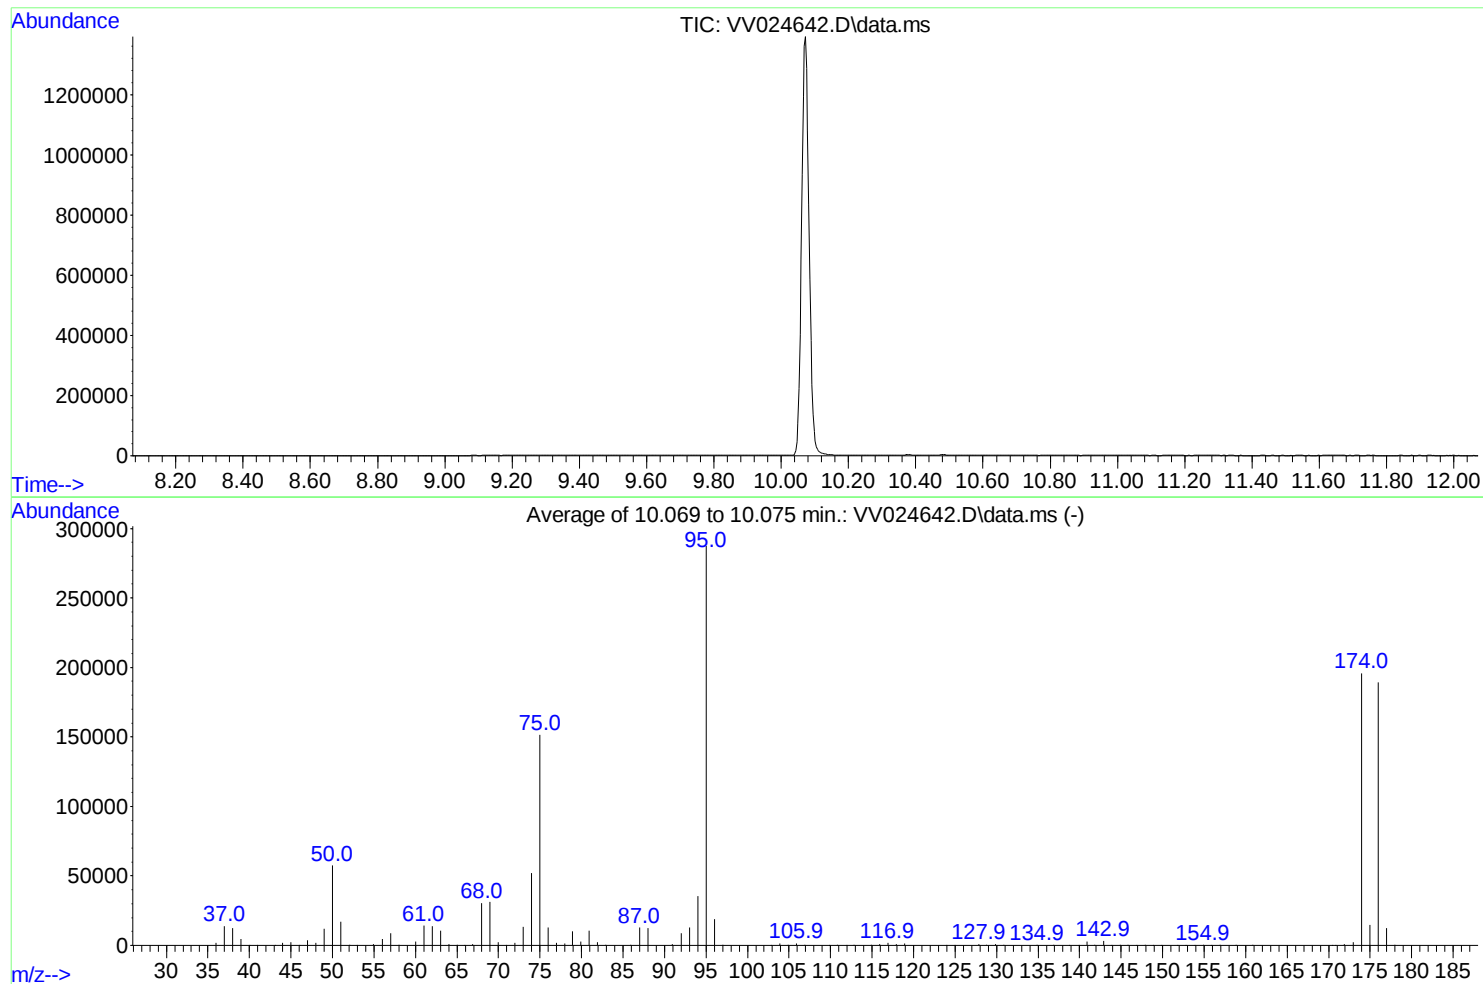

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	57389	PASS
75	95	30	80	52.7	151467	PASS
95	95	100	100	100.0	287253	PASS
96	95	5	9	6.6	19032	PASS
173	174	0.00	2	1.1	2235	PASS
174	95	50	120	68.2	195925	PASS
175	174	5	9	7.5	14646	PASS
176	174	95	105	96.6	189269	PASS
177	176	5	10	6.6	12404	PASS

m/z	Abundance
35.90	916.0
37.90	369.0
40.00	128.0
43.90	264.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	3054.0
37.00	14425.0
38.00	13494.0
39.00	4821.0
40.00	252.0
40.90	106.0
43.10	166.0
44.00	2057.0
45.00	2523.0
45.90	240.0
47.00	3661.0
48.00	1757.0
49.00	12776.0
50.00	59472.0
51.00	17360.0
52.00	697.0
52.90	122.0
55.00	827.0
56.00	4752.0
57.00	8734.0
58.00	341.0
60.00	2609.0
61.00	14558.0
62.00	13946.0
63.00	10973.0
64.00	1148.0
65.00	551.0
65.90	147.0
66.90	813.0
68.00	30832.0
69.00	32088.0
70.00	2474.0
70.90	103.0
72.00	1763.0
73.00	13615.0
74.00	53448.0
75.00	154496.0
76.00	13633.0
77.00	1975.0
77.90	1171.0
78.90	10051.0
79.90	2702.0
80.90	11003.0
81.90	2385.0
82.90	270.0
85.90	426.0
87.00	12649.0
88.00	12692.0
90.90	1090.0
92.00	8838.0
93.00	13359.0
94.00	35648.0
95.00	290624.0
96.00	19640.0
97.00	598.0
102.80	175.0
103.90	1443.0
104.90	502.0
105.90	1604.0
106.90	261.0
109.80	224.0
110.80	273.0
111.90	201.0
112.90	253.0
115.00	368.0
115.90	1216.0
116.90	1873.0
117.90	1216.0
118.90	1618.0
123.90	176.0
124.90	105.0
127.90	1147.0
128.80	453.0
129.90	965.0
130.90	352.0
134.90	503.0
136.80	443.0
138.80	116.0
139.90	222.0
140.90	2866.0
141.80	378.0
142.90	3128.0
143.90	212.0
144.90	347.0
145.80	387.0
146.90	220.0
147.90	561.0
148.80	192.0
149.80	219.0
151.80	154.0
152.80	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

153.80	144.0
154.90	630.0
155.80	171.0
156.90	456.0
158.80	345.0
160.90	328.0
170.80	149.0
171.90	851.0
173.00	2165.0
174.00	193344.0
175.00	14733.0
176.00	186880.0
177.00	12552.0
178.00	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	2978.0
37.00	14431.0
38.00	13355.0
39.00	4836.0
40.00	259.0
40.90	104.0
43.00	169.0
44.00	2013.0
45.00	2515.0
46.00	221.0
47.00	3580.0
48.00	1776.0
49.00	12420.0
50.00	59456.0
51.00	17320.0
52.10	712.0
54.90	784.0
56.00	4614.0
57.00	8836.0
58.00	345.0
60.00	2639.0
61.00	14620.0
62.00	13979.0
63.00	11081.0
64.00	1146.0
65.00	431.0
65.90	139.0
66.90	818.0
68.00	31584.0
69.00	32448.0
70.00	2497.0
70.90	109.0
72.00	1750.0
73.00	13798.0
74.00	53936.0
75.00	156352.0
76.00	13487.0
77.00	1881.0
78.00	1251.0
78.90	10252.0
79.90	2721.0
80.90	11130.0
81.90	2430.0
83.00	304.0
85.90	417.0
87.00	13261.0
88.00	12941.0
90.90	1074.0
92.00	9068.0
93.00	13255.0
94.00	36584.0
95.00	296896.0
96.00	19672.0
97.00	510.0
102.80	177.0
103.90	1375.0
104.90	450.0
105.90	1612.0
106.90	267.0
109.80	232.0
110.80	277.0
111.90	261.0
112.80	294.0
114.90	352.0
115.90	1216.0
116.90	1930.0
117.90	1192.0
118.90	1633.0
123.90	201.0
124.90	141.0
127.90	1074.0
128.80	492.0
129.90	997.0
130.80	393.0
134.90	610.0
136.90	451.0
138.70	119.0
139.90	267.0
140.90	2913.0
141.80	402.0
142.90	3221.0
143.80	183.0
144.90	360.0
145.80	429.0
146.90	226.0
147.90	580.0
148.80	177.0
149.80	201.0
151.80	189.0
152.80	201.0
153.80	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

154.90	677.0
155.80	187.0
156.90	496.0
158.80	404.0
160.80	344.0
170.50	147.0
171.90	775.0
173.00	2272.0
174.00	202752.0
175.00	15091.0
176.00	195968.0
177.00	12799.0
178.00	315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

m/z	Abundance
36.00	2762.0
37.00	13039.0
38.00	11694.0
39.00	4347.0
40.00	238.0
43.00	155.0
44.00	1852.0
45.00	2263.0
46.10	225.0
47.00	3206.0
48.00	1585.0
49.00	10872.0
50.00	53240.0
51.00	15913.0
52.00	705.0
54.90	741.0
56.00	4195.0
57.00	8154.0
58.00	304.0
60.00	2515.0
61.00	13273.0
62.00	12952.0
63.00	10206.0
64.00	1045.0
65.00	331.0
65.90	106.0
66.90	762.0
68.00	29096.0
69.00	29656.0
70.00	2221.0
71.90	1608.0
73.00	12714.0
74.00	48720.0
75.00	143552.0
76.00	12086.0
77.00	1594.0
78.00	1157.0
78.90	9558.0
79.90	2536.0
80.90	10139.0
81.90	2328.0
83.00	290.0
86.00	344.0
87.00	12307.0
88.00	11990.0
90.90	1040.0
92.00	8573.0
93.00	11854.0
94.00	33720.0
95.00	274240.0
96.00	17784.0
97.00	394.0
102.80	140.0
103.90	1235.0
104.90	373.0
105.90	1352.0
106.90	271.0
109.80	223.0
110.80	259.0
111.90	264.0
112.80	331.0
114.90	277.0
115.90	1000.0
116.90	1751.0
117.90	1040.0
118.90	1502.0
123.90	196.0
124.90	140.0
127.90	920.0
128.80	493.0
129.90	938.0
130.80	439.0
134.90	591.0
136.90	452.0
138.70	120.0
139.90	266.0
140.90	2712.0
141.80	335.0
142.90	2961.0
143.70	164.0
144.90	307.0
145.80	401.0
146.80	225.0
147.90	538.0
148.80	138.0
149.80	189.0
151.80	191.0
152.80	184.0
153.90	159.0
154.90	663.0
155.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269

156.90	456.0
158.90	411.0
160.80	318.0
170.30	150.0
171.90	641.0
173.00	2269.0
174.00	191680.0
175.00	14114.0
176.00	184960.0
177.00	11861.0
178.00	322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB269