

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021424\
 Data File : VW034171.D
 Acq On : 14 Feb 2024 10:58
 Operator : SY/MD
 Sample : P1455-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Quant Time: Feb 15 01:28:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 15 01:26:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	85539	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	78191	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	39061	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	21963	3.315	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.400%
7) Chloroethane-d5	1.535	69	20180	3.478	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.600%
11) 1,1-Dichloroethene-d2	2.060	65	11380	3.562	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.200%
20) 2-Butanone-d5	3.815	46	37459	33.668	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	67.340%
24) Chloroform-d	4.252	84	46670	3.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.600%
26) 1,2-Dichloroethane-d4	4.944	65	23065	4.100	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.000%
32) Benzene-d6	4.963	84	87287	3.721	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.400%
36) 1,2-Dichloropropane-d6	5.989	67	23825	3.633	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.600%
41) Toluene-d8	7.246	98	79924	3.707	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	7.561	79	9406	3.799	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.000%
46) 2-Hexanone-d5	8.030	63	28062	31.747	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	63.500%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	14359	3.612	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.200%
66) 1,2-Dichlorobenzene-d4	11.561	152	28695	4.039	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	80.800%
Target Compounds					Qvalue	
13) Acetone	2.140	43	5047	5.979	ug/L	# 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034171.D
Acq On : 14 Feb 2024 10:58
Operator : SY/MD
Sample : P1455-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAH1

Quant Time: Feb 15 01:28:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 15 01:26:50 2024
Response via : Initial Calibration

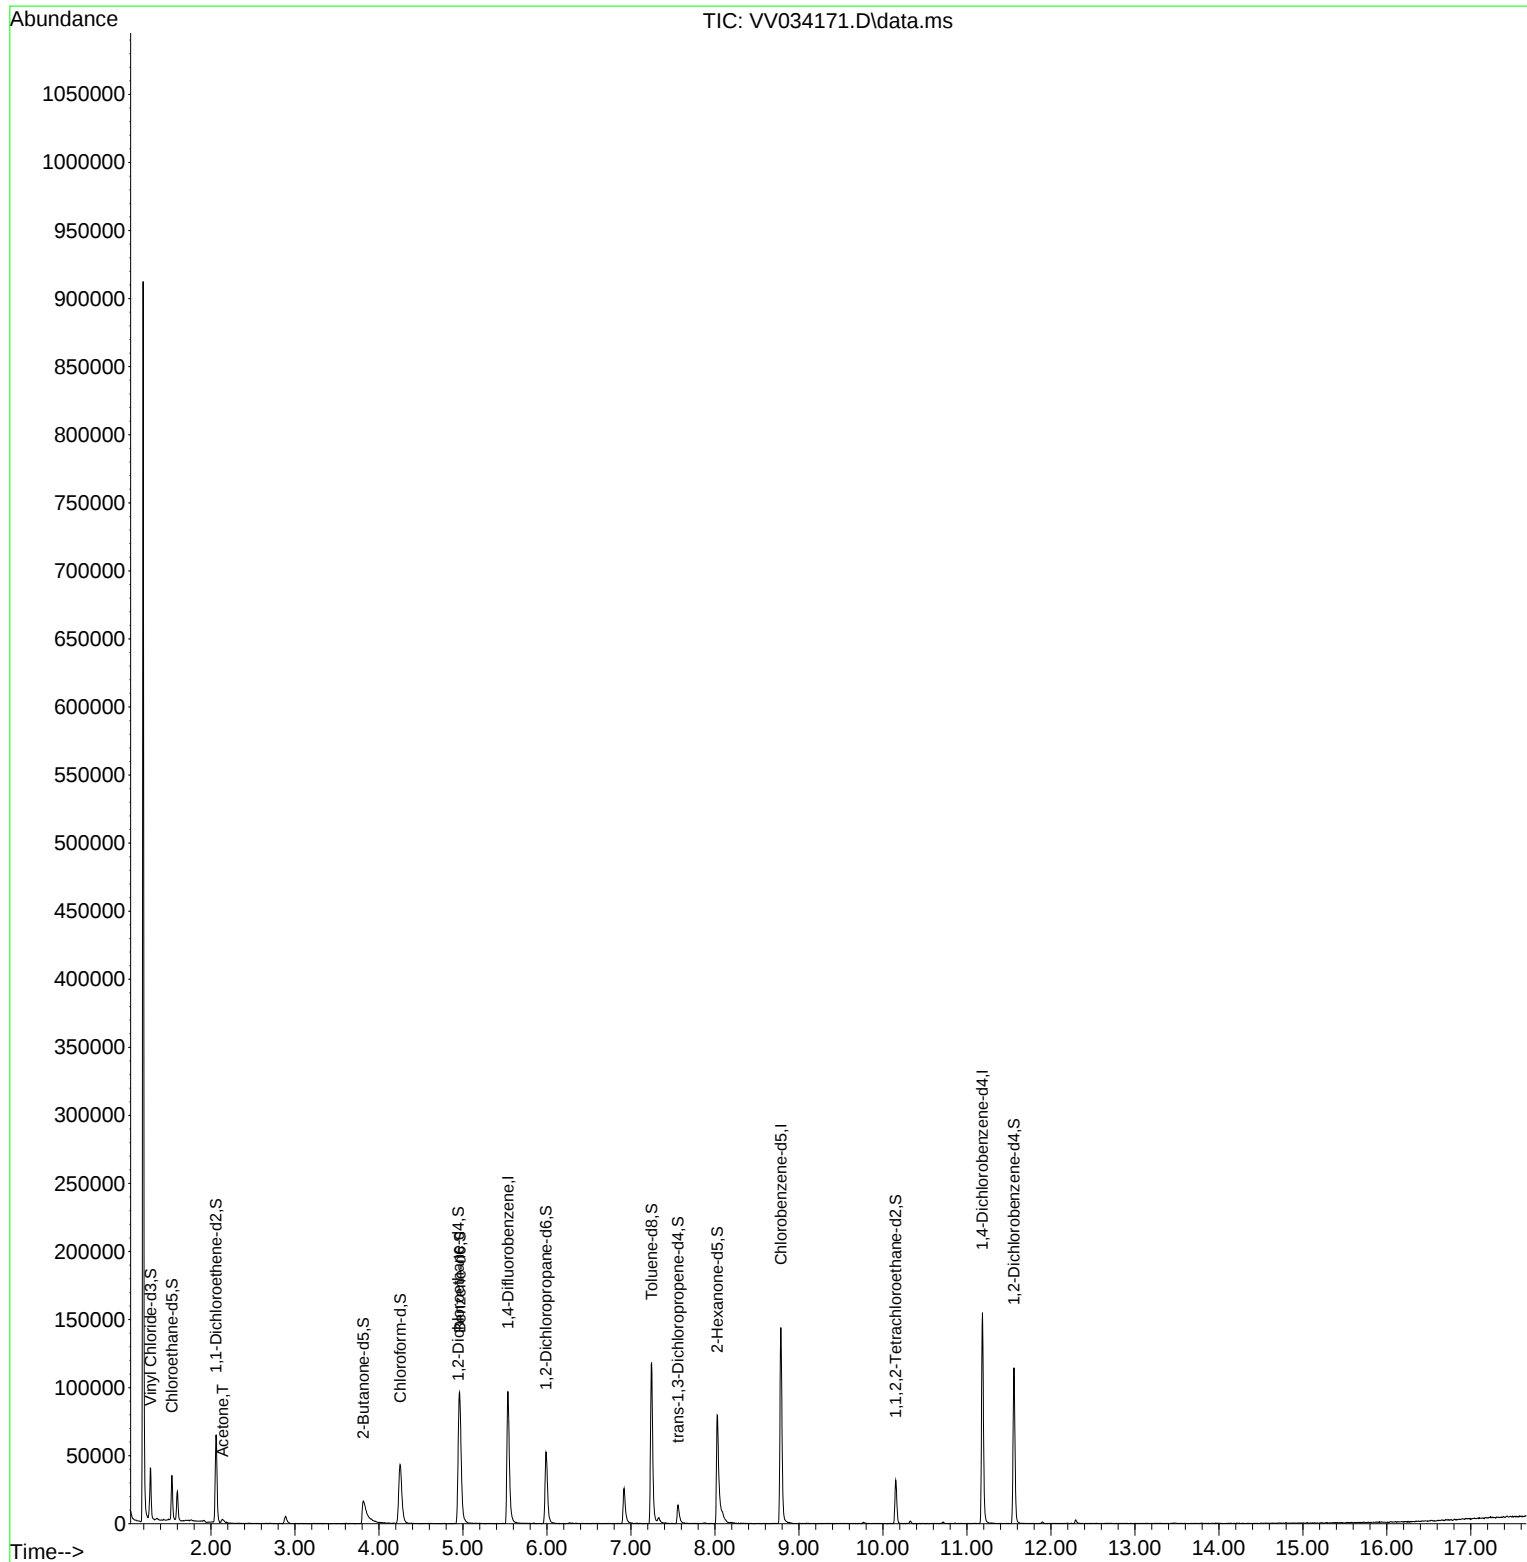

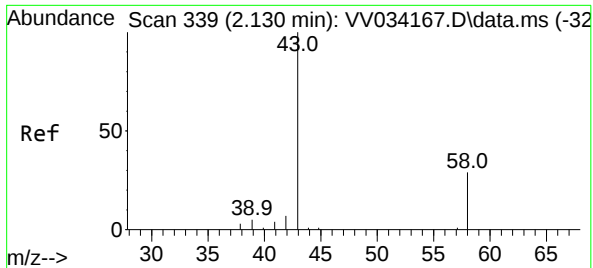

#13
 Acetone
 Concen: 5.979 ug/L
 RT: 2.140 min Scan# 34
 Delta R.T. 0.010 min
 Lab File: VV034171.D
 Acq: 14 Feb 2024 10:58

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH1

Tgt Ion: 43 Resp: 5047
 Ion Ratio Lower Upper
 43 100
 58 22.7 0.0 13.8#

