

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034168.D
 Acq On : 14 Feb 2024 09:42
 Operator : SY/MD
 Sample : VV0214WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	39	45	51	rBV	2672	4163	1.73%	0.216%
2	1.281	68	75	92	rVB	35746	40336	16.77%	2.097%
3	1.535	146	154	171	rVB	36331	43637	18.15%	2.268%
4	2.059	308	317	332	rVB	66424	96841	40.27%	5.033%
5	2.452	431	439	447	rBV3	1989	2915	1.21%	0.152%
6	3.805	849	860	893	rBV2	21601	70719	29.41%	3.676%
7	4.252	983	999	1030	rVB2	42487	111788	46.48%	5.810%
8	4.960	1205	1219	1248	rBV3	95026	240490	100.00%	12.500%
9	5.535	1388	1398	1422	rBV2	80187	163053	67.80%	8.475%
10	5.992	1528	1540	1567	rBV	53627	111857	46.51%	5.814%
11	6.918	1818	1828	1848	rBV2	23351	46231	19.22%	2.403%
12	7.246	1919	1930	1956	rBV	113747	202905	84.37%	10.546%
13	7.561	2019	2028	2047	rBV2	13157	24464	10.17%	1.272%
14	8.027	2163	2173	2216	rBV	81872	175712	73.06%	9.133%
15	8.368	2270	2279	2289	rBV3	2731	4604	1.91%	0.239%
16	8.786	2399	2409	2434	rBV	115085	191550	79.65%	9.956%
17	10.156	2824	2835	2850	rBV2	31433	50282	20.91%	2.613%
18	11.185	3144	3155	3176	rBV	113939	181206	75.35%	9.418%
19	11.561	3261	3272	3294	rBV	101253	161215	67.04%	8.379%




Sum of corrected areas: 1923968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034168.D
Acq On : 14 Feb 2024 09:42
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

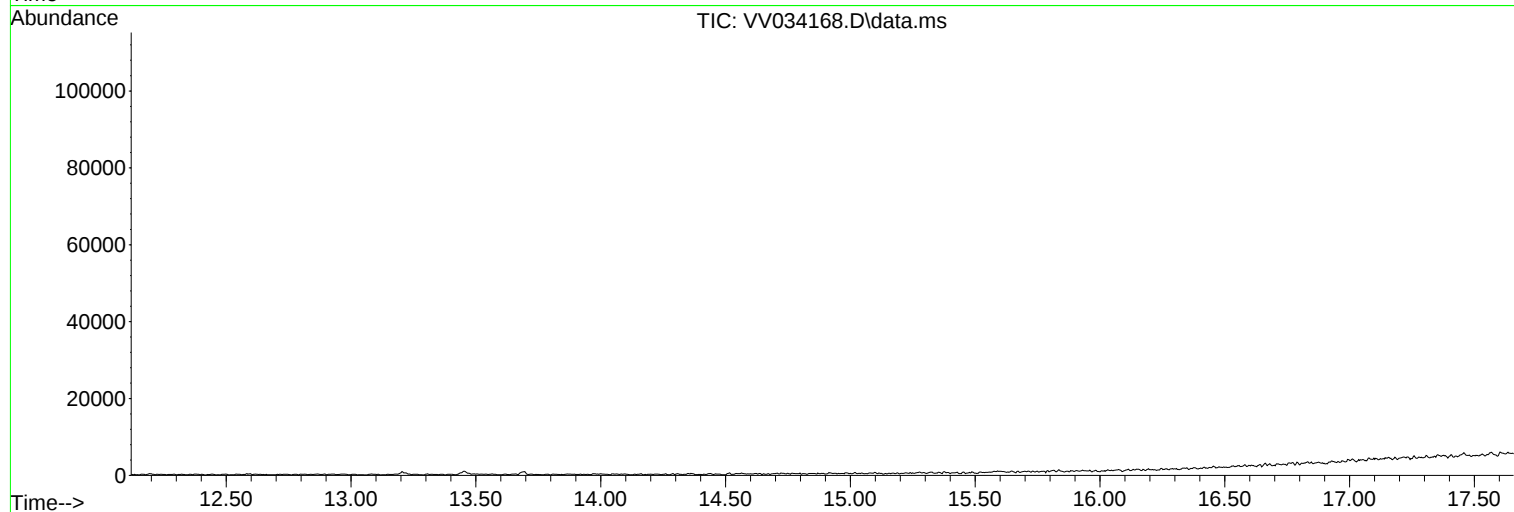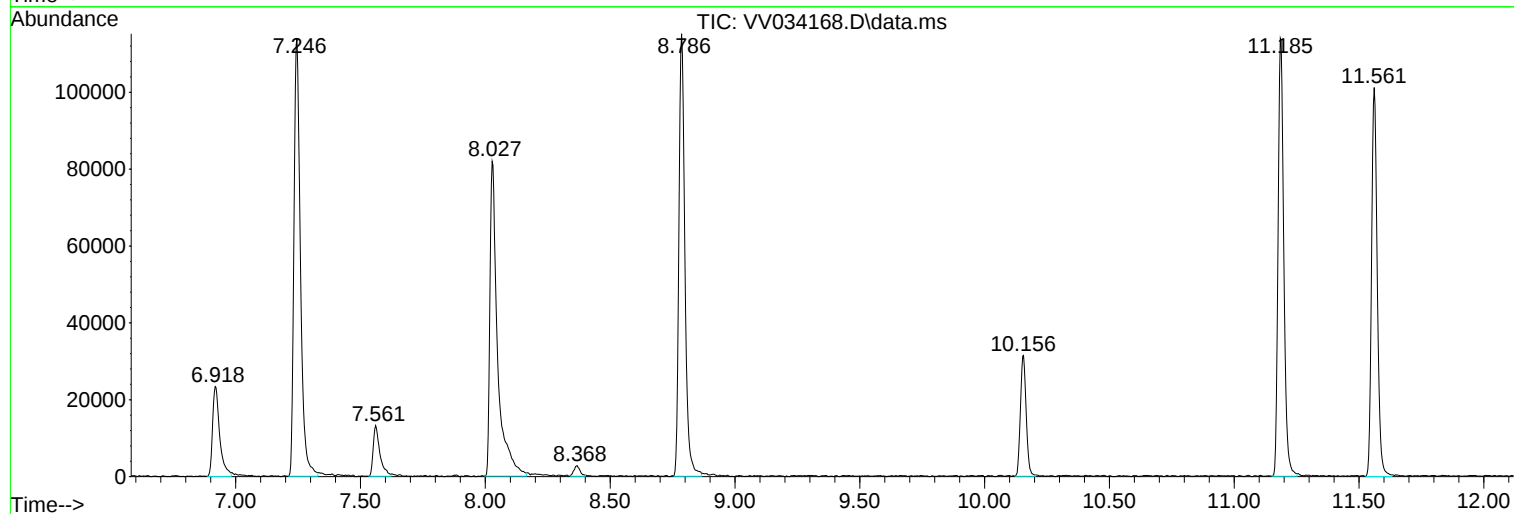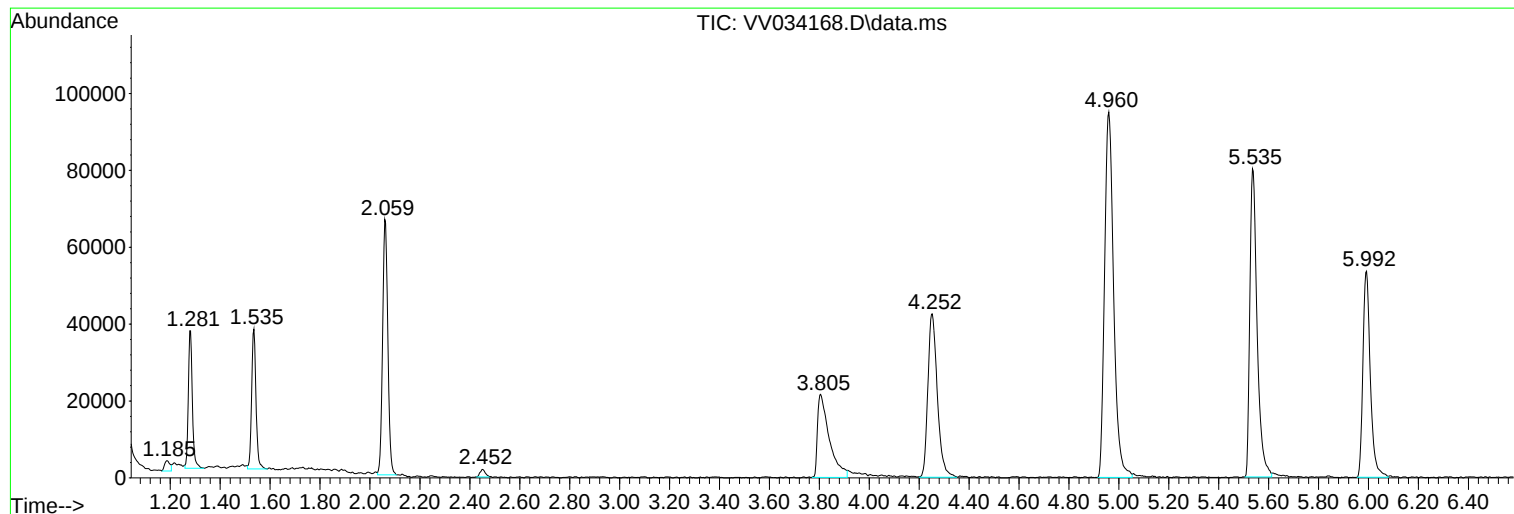

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034168.D
Acq On : 14 Feb 2024 09:42
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034168.D
Acq On : 14 Feb 2024 09:42
Operator : SY/MD
Sample : VV0214WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc