

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034169.D
 Acq On : 14 Feb 2024 10:11
 Operator : SY/MD
 Sample : P1402-08DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	33281	37478	10.11%	1.186%
2	1.535	146	154	165	rBV	31579	37115	10.01%	1.174%
3	2.069	307	320	341	rVB4	217526	352047	94.99%	11.137%
4	3.114	630	645	665	rBV	21238	45606	12.31%	1.443%
5	3.815	851	863	893	rBV3	75926	202542	54.65%	6.407%
6	4.249	984	998	1022	rBV	40813	105445	28.45%	3.336%
7	4.510	1066	1079	1096	rBV4	7887	18615	5.02%	0.589%
8	4.957	1205	1218	1244	rBV2	89533	223643	60.34%	7.075%
9	5.532	1386	1397	1426	rBV	112099	234279	63.21%	7.411%
10	5.831	1479	1490	1518	rBV2	108337	222389	60.00%	7.035%
11	5.989	1527	1539	1561	rBV	48360	102455	27.64%	3.241%
12	6.918	1818	1828	1849	rBV2	24063	45797	12.36%	1.449%
13	7.243	1918	1929	1957	rBV	112001	201881	54.47%	6.386%
14	7.561	2019	2028	2043	rBV	11688	23029	6.21%	0.728%
15	7.902	2119	2134	2158	rBV	215337	370627	100.00%	11.724%
16	8.027	2164	2173	2207	rBV	74757	161498	43.57%	5.109%
17	8.783	2397	2408	2428	rBV	169428	281155	75.86%	8.894%
18	10.153	2824	2834	2844	rBV	29082	45695	12.33%	1.445%
19	11.185	3145	3155	3181	rBV	182449	282992	76.35%	8.952%
20	11.561	3261	3272	3290	rBV	104893	166904	45.03%	5.280%




Sum of corrected areas: 3161192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034169.D
Acq On : 14 Feb 2024 10:11
Operator : SY/MD
Sample : P1402-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

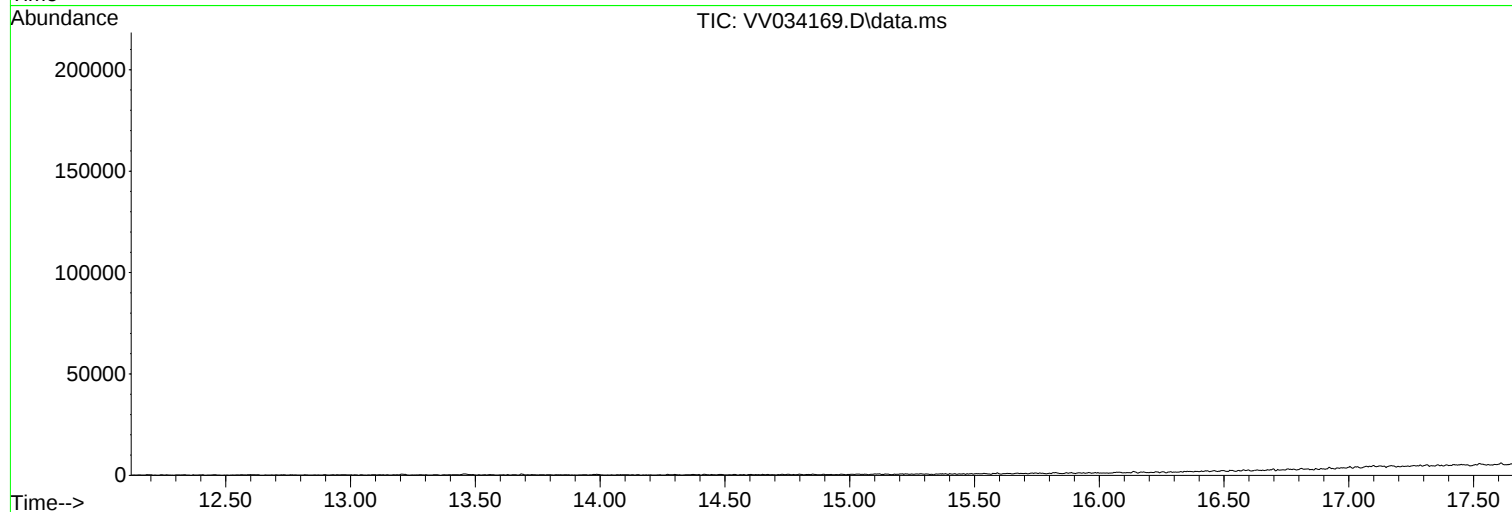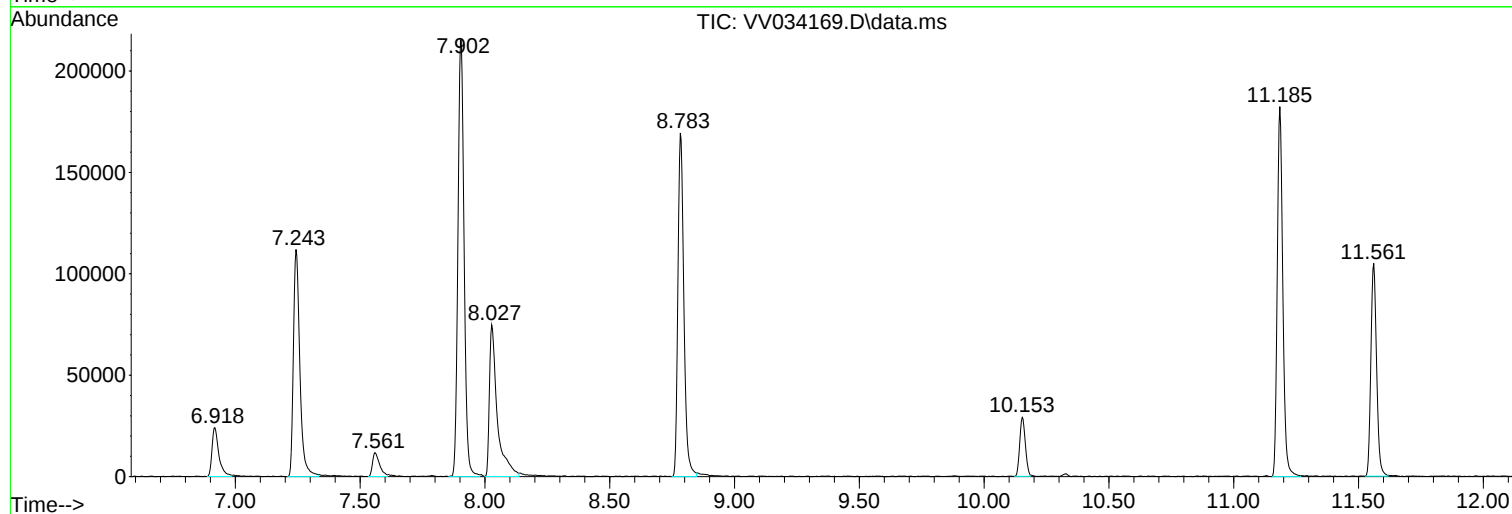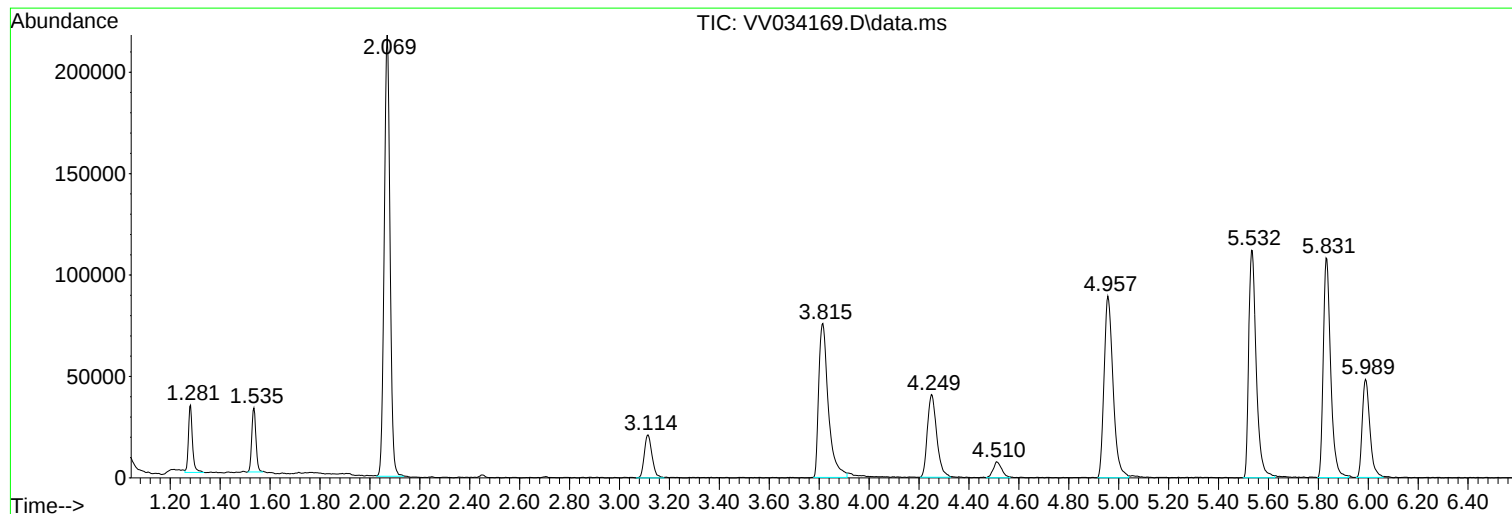

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034169.D
Acq On : 14 Feb 2024 10:11
Operator : SY/MD
Sample : P1402-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034169.D
Acq On : 14 Feb 2024 10:11
Operator : SY/MD
Sample : P1402-08DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc