

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034173.D
 Acq On : 14 Feb 2024 11:46
 Operator : SY/MD
 Sample : P1455-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	90	rVB2	36722	49780	20.24%	2.351%
2	1.536	146	154	169	rVB	34583	41655	16.94%	1.967%
3	2.060	306	317	332	rBV	66246	97307	39.56%	4.596%
4	2.140	332	342	357	rBV3	3134	8219	3.34%	0.388%
5	3.600	782	796	814	rBV3	6061	15324	6.23%	0.724%
6	3.818	853	864	900	rBV2	16799	67167	27.31%	3.172%
7	4.249	983	998	1023	rBV2	43468	112181	45.61%	5.298%
8	4.960	1205	1219	1248	rBV3	98534	245954	100.00%	11.616%
9	5.535	1388	1398	1423	rBV2	85389	178226	72.46%	8.417%
10	5.989	1524	1539	1561	rBV2	53604	112728	45.83%	5.324%
11	6.461	1676	1686	1700	rBV6	2980	6516	2.65%	0.308%
12	6.918	1819	1828	1845	rBV	26456	50158	20.39%	2.369%
13	7.243	1917	1929	1956	rBV	118681	215489	87.61%	10.177%
14	7.558	2019	2027	2047	rBV	14053	26654	10.84%	1.259%
15	8.027	2165	2173	2209	rBV	89778	194696	79.16%	9.195%
16	8.786	2399	2409	2435	rBV	132070	220635	89.71%	10.420%
17	10.153	2825	2834	2854	rBV	34188	53911	21.92%	2.546%
18	10.886	3054	3062	3075	rBV2	2993	6129	2.49%	0.289%
19	11.185	3145	3155	3174	rBV	143314	221112	89.90%	10.443%
20	11.561	3261	3272	3292	rBV2	117866	187212	76.12%	8.842%
21	12.294	3492	3500	3512	rVB3	4276	6331	2.57%	0.299%




Sum of corrected areas: 2117384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034173.D
Acq On : 14 Feb 2024 11:46
Operator : SY/MD
Sample : P1455-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

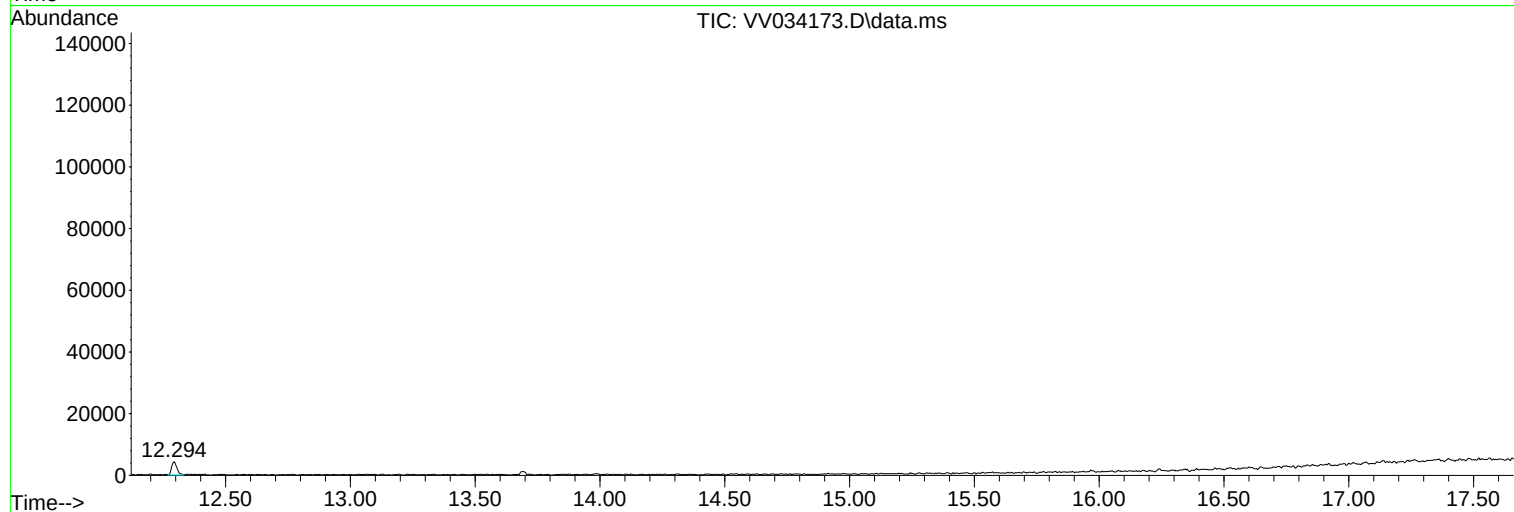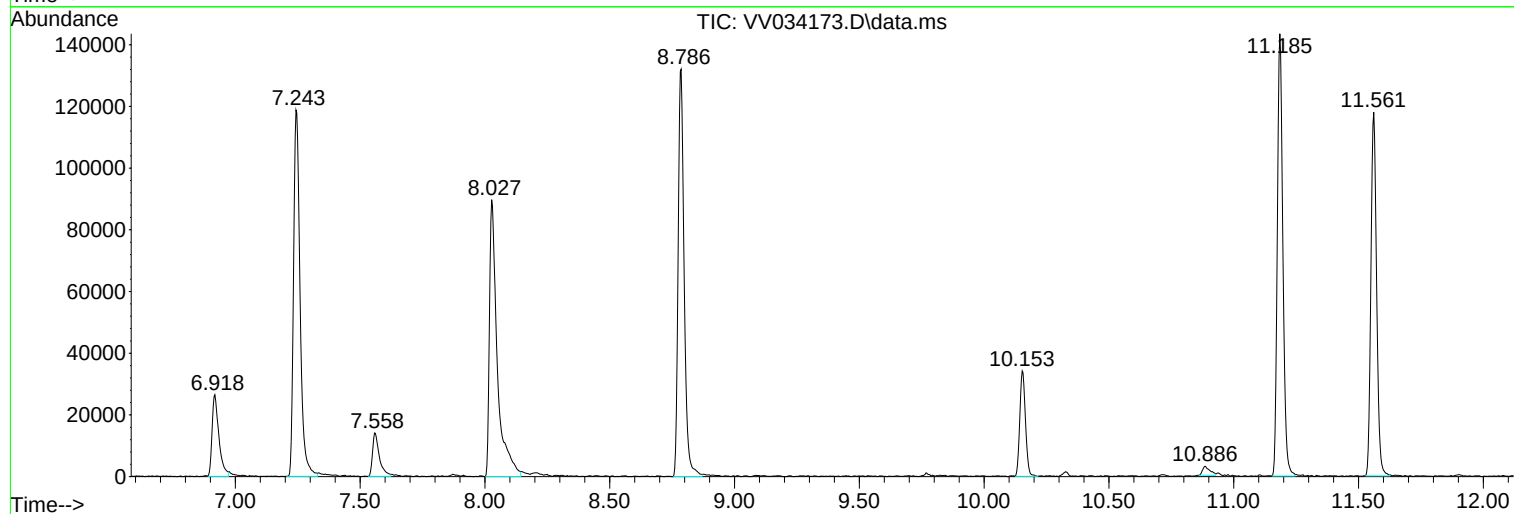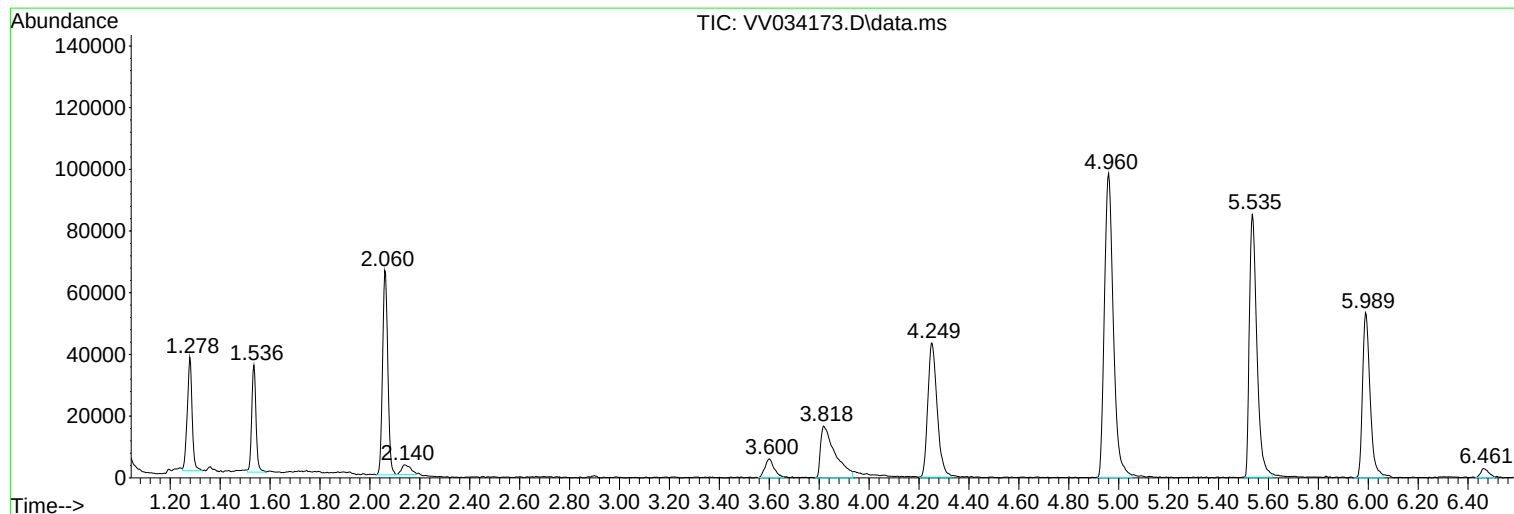

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034173.D
Acq On : 14 Feb 2024 11:46
Operator : SY/MD
Sample : P1455-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034173.D
Acq On : 14 Feb 2024 11:46
Operator : SY/MD
Sample : P1455-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
