

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034175.D
 Acq On : 14 Feb 2024 12:33
 Operator : SY/MD
 Sample : P1455-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	84	rBV	32176	33691	14.04%	1.397%
2	1.536	146	154	166	rVB	31786	36568	15.24%	1.516%
3	2.063	308	318	335	rBV2	70985	110204	45.92%	4.569%
4	3.812	851	862	893	rBV2	26699	85764	35.73%	3.556%
5	4.252	984	999	1026	rBV2	44245	125108	52.13%	5.187%
6	4.738	1135	1150	1176	rBV2	24356	60414	25.17%	2.505%
7	4.960	1204	1219	1244	rBV2	95731	240009	100.00%	9.951%
8	5.535	1388	1398	1429	rBV	87789	180862	75.36%	7.499%
9	5.838	1481	1492	1517	rBV2	45953	95969	39.99%	3.979%
10	5.992	1527	1540	1565	rBV	53269	111946	46.64%	4.642%
11	6.918	1819	1828	1853	rBV	25444	49491	20.62%	2.052%
12	7.243	1919	1929	1954	rBV	115643	209803	87.41%	8.699%
13	7.561	2020	2028	2048	rBV2	13727	25784	10.74%	1.069%
14	7.905	2124	2135	2159	rVB	101261	171515	71.46%	7.111%
15	8.027	2165	2173	2211	rBV	91810	192962	80.40%	8.001%
16	8.786	2398	2409	2433	rBV	129051	218439	91.01%	9.057%
17	10.153	2825	2834	2845	rBV2	33821	53440	22.27%	2.216%
18	10.326	2879	2888	2897	rVB	1987	3174	1.32%	0.132%
19	11.185	3144	3155	3177	rBV	143656	223078	92.95%	9.249%
20	11.561	3262	3272	3290	rBV	117991	183603	76.50%	7.613%




Sum of corrected areas: 2411824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034175.D
Acq On : 14 Feb 2024 12:33
Operator : SY/MD
Sample : P1455-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

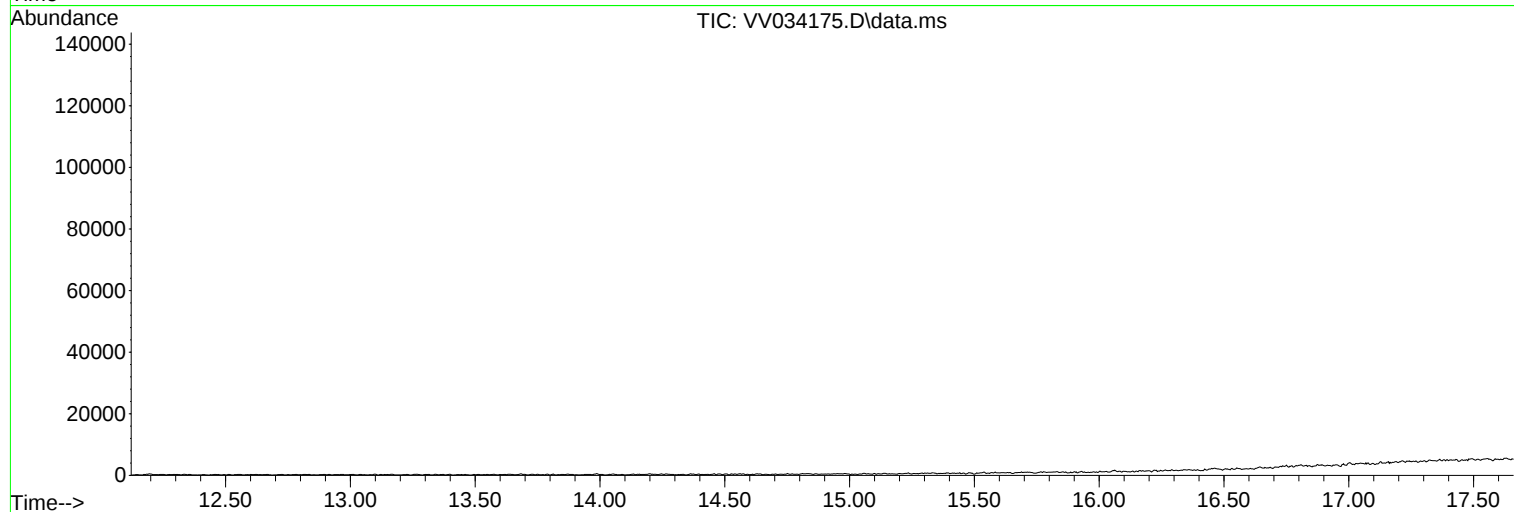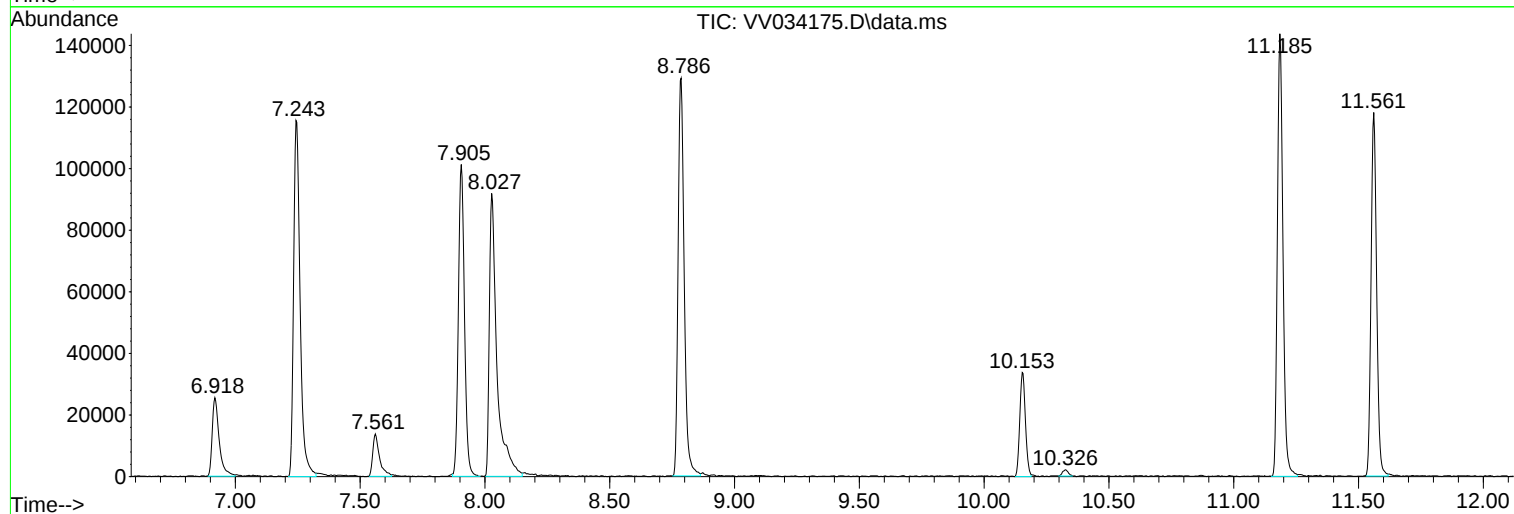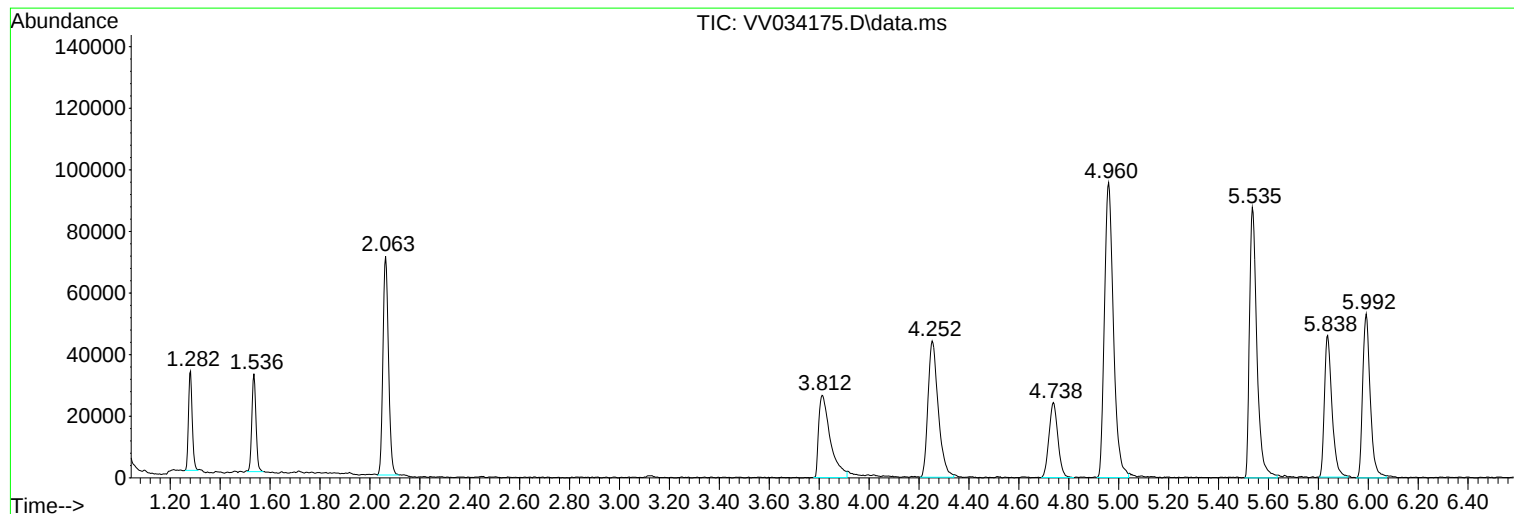

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034175.D
Acq On : 14 Feb 2024 12:33
Operator : SY/MD
Sample : P1455-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034175.D
Acq On : 14 Feb 2024 12:33
Operator : SY/MD
Sample : P1455-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------