

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034176.D
 Acq On : 14 Feb 2024 12:57
 Operator : SY/MD
 Sample : P1455-01DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	31916	35004	14.66%	1.516%
2	1.536	146	154	166	rVB	31995	37779	15.83%	1.636%
3	2.063	307	318	334	rVB2	64919	97367	40.79%	4.216%
4	2.449	431	438	447	rBV3	4676	7599	3.18%	0.329%
5	3.815	854	863	898	rBV3	26072	87131	36.50%	3.773%
6	4.253	983	999	1028	rBV	42245	109766	45.98%	4.753%
7	4.960	1202	1219	1245	rBV2	94786	238714	100.00%	10.336%
8	5.535	1388	1398	1428	rBV	89336	182583	76.49%	7.906%
9	5.834	1480	1491	1522	rBV2	109065	220520	92.38%	9.549%
10	5.992	1528	1540	1565	rBV	52466	109111	45.71%	4.725%
11	6.918	1819	1828	1855	rBV	25694	49675	20.81%	2.151%
12	7.243	1919	1929	1958	rBV	115777	210041	87.99%	9.095%
13	7.561	2019	2028	2048	rBV	14011	26105	10.94%	1.130%
14	7.908	2127	2136	2151	rVB3	13079	23099	9.68%	1.000%
15	8.027	2165	2173	2214	rBV	88012	192557	80.66%	8.338%
16	8.786	2399	2409	2431	rBV	131461	223277	93.53%	9.668%
17	10.153	2825	2834	2847	rBV2	33980	52742	22.09%	2.284%
18	11.185	3145	3155	3179	rBV	145893	224918	94.22%	9.739%
19	11.561	3261	3272	3295	rVB	113129	181445	76.01%	7.857%




Sum of corrected areas: 2309433

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034176.D
Acq On : 14 Feb 2024 12:57
Operator : SY/MD
Sample : P1455-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

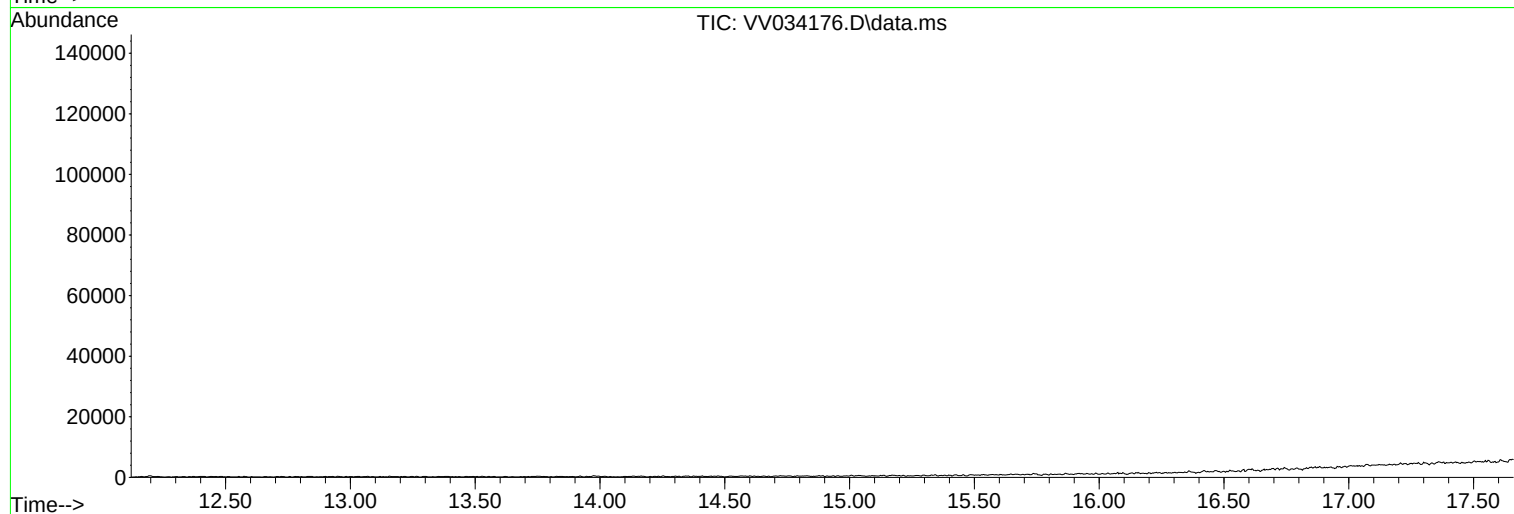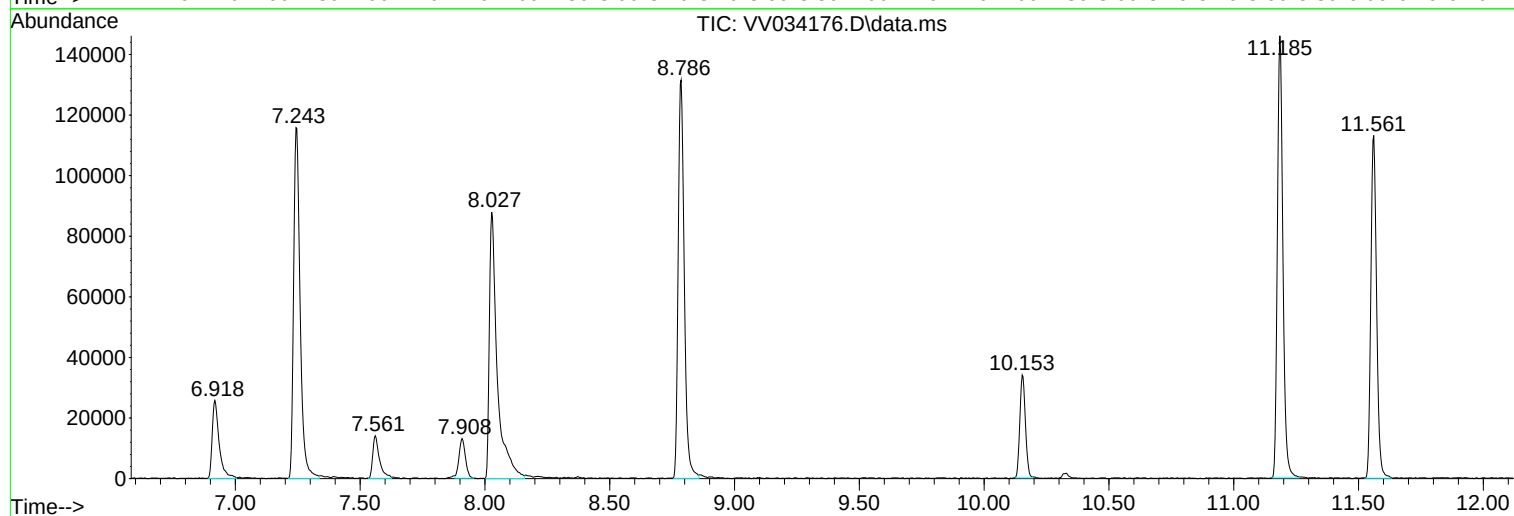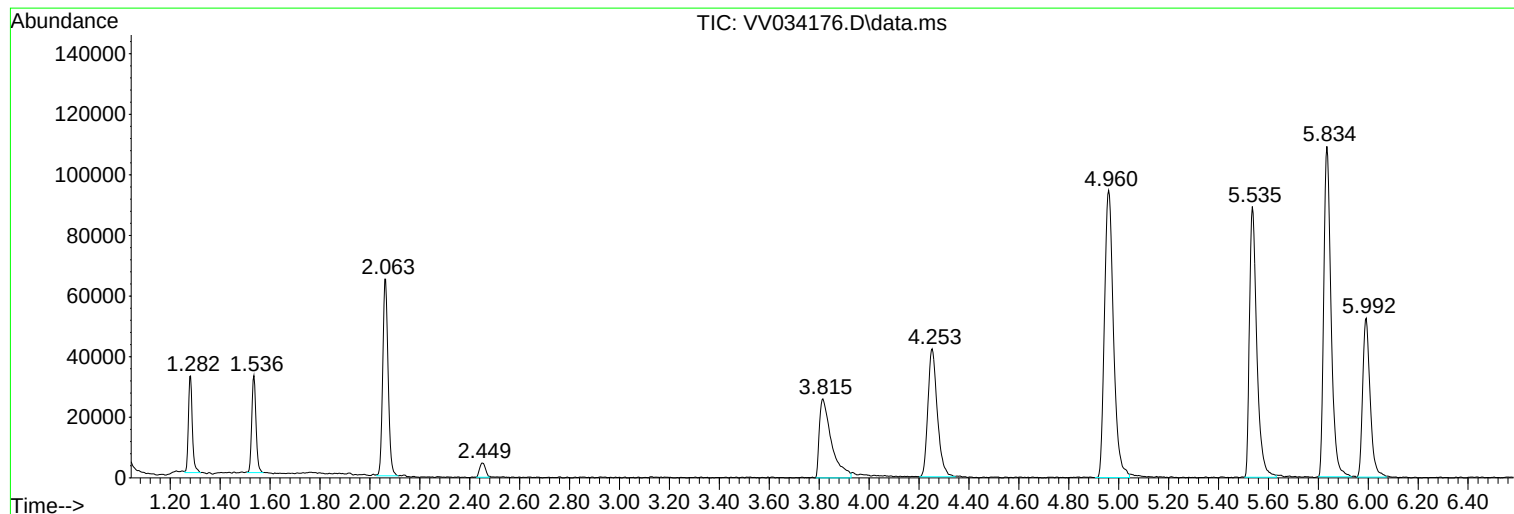

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034176.D
Acq On : 14 Feb 2024 12:57
Operator : SY/MD
Sample : P1455-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034176.D
Acq On : 14 Feb 2024 12:57
Operator : SY/MD
Sample : P1455-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc