

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
 Data File : VV034178.D
 Acq On : 14 Feb 2024 13:51
 Operator : SY/MD
 Sample : P1455-02DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	94	rVB	33280	35903	9.55%	1.486%
2	1.536	146	154	163	rBV	30812	35842	9.53%	1.484%
3	2.060	307	317	332	rBV	63407	92977	24.72%	3.849%
4	2.452	427	439	451	rVB2	6694	11143	2.96%	0.461%
5	3.818	855	864	908	rBV2	24230	88151	23.44%	3.649%
6	4.252	985	999	1021	rBV	41574	107831	28.67%	4.464%
7	4.960	1204	1219	1251	rBV2	94545	238753	63.48%	9.884%
8	5.535	1387	1398	1433	rBV	83421	174826	46.48%	7.238%
9	5.834	1479	1491	1519	rBV	184162	376107	100.00%	15.570%
10	5.989	1528	1539	1561	rBV2	51621	106289	28.26%	4.400%
11	6.918	1819	1828	1846	rBV2	25475	47938	12.75%	1.985%
12	7.246	1919	1930	1957	rBV	114864	208947	55.56%	8.650%
13	7.561	2018	2028	2051	rBV2	12988	26724	7.11%	1.106%
14	7.912	2130	2137	2150	rVB3	4310	6959	1.85%	0.288%
15	8.030	2164	2174	2212	rBV	89271	193280	51.39%	8.001%
16	8.786	2398	2409	2435	rBV	129812	212495	56.50%	8.797%
17	10.153	2825	2834	2848	rBV	33736	53583	14.25%	2.218%
18	11.185	3145	3155	3177	rBV	135947	215933	57.41%	8.939%
19	11.561	3260	3272	3294	rBV	114720	181871	48.36%	7.529%




Sum of corrected areas: 2415552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034178.D
Acq On : 14 Feb 2024 13:51
Operator : SY/MD
Sample : P1455-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

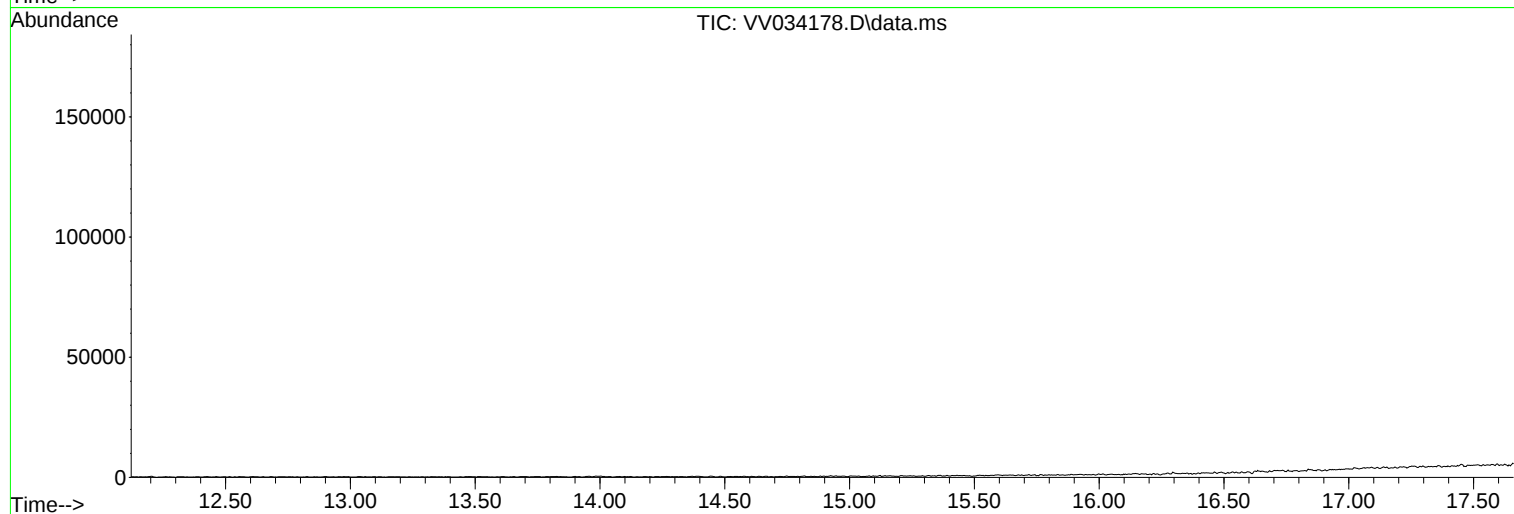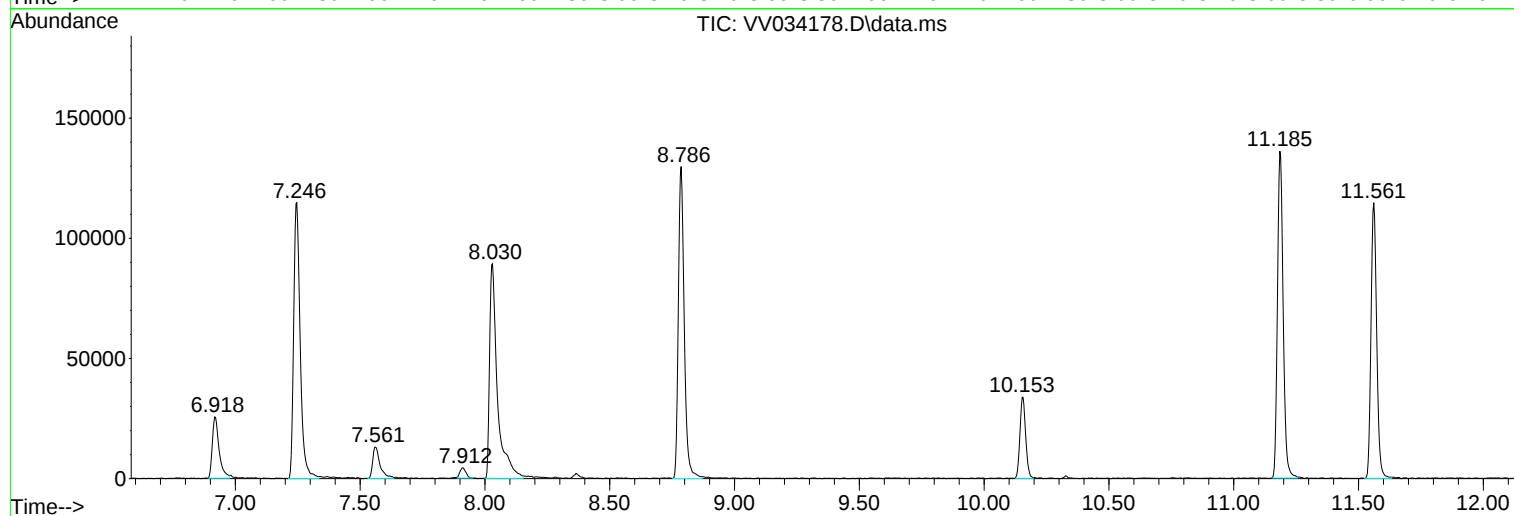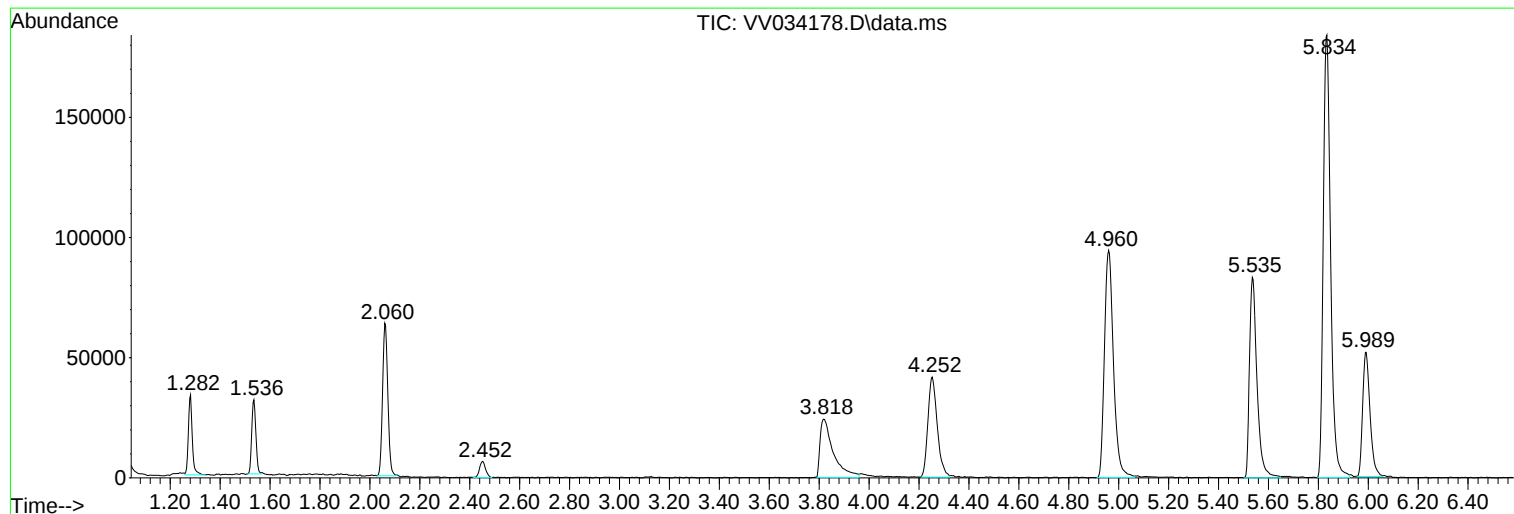

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034178.D
Acq On : 14 Feb 2024 13:51
Operator : SY/MD
Sample : P1455-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021424\
Data File : VV034178.D
Acq On : 14 Feb 2024 13:51
Operator : SY/MD
Sample : P1455-02DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc