
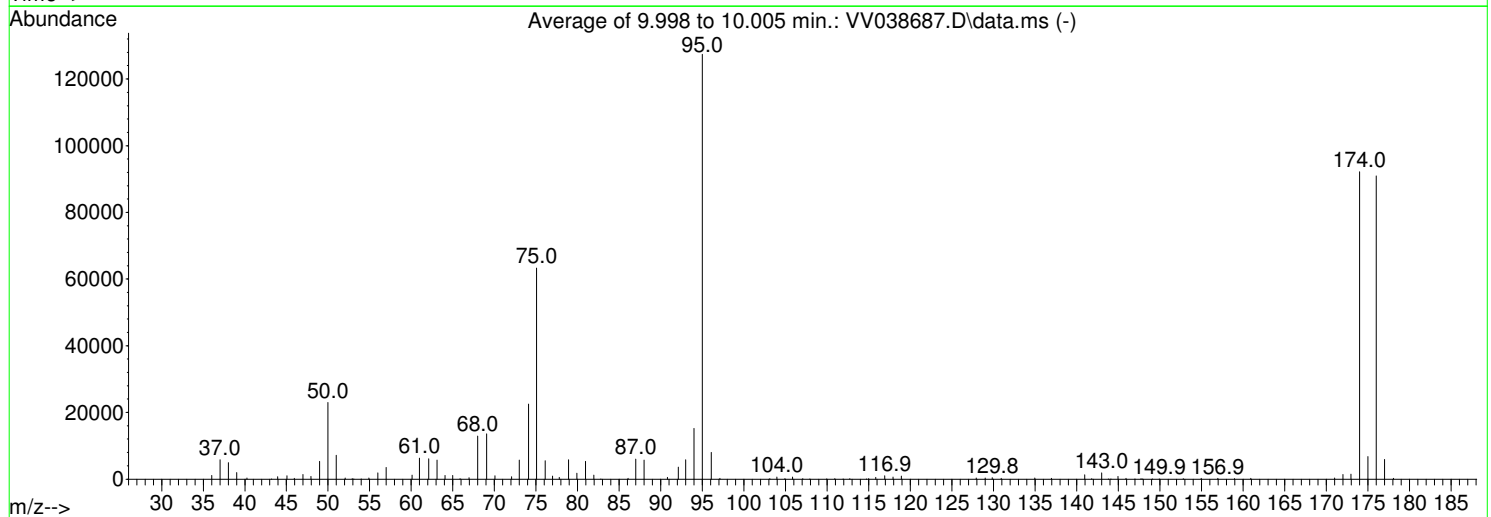


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV021425\
Data File : VV038687.D
Acq On : 14 Feb 2025 08:55
Operator : SY/MD
Sample : BFB205
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 17 10:31:04 2025

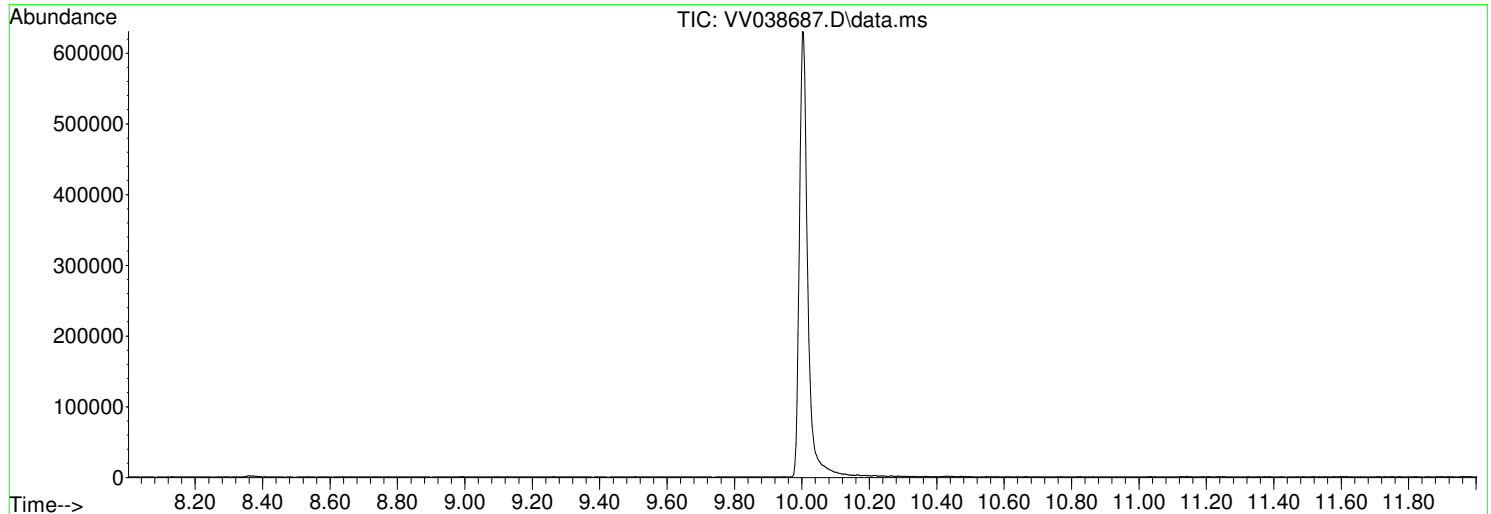

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	22957	PASS
75	95	30	80	49.7	63349	PASS
95	95	100	100	100.0	127416	PASS
96	95	5	9	6.3	8045	PASS
173	174	0.00	2	1.7	1532	PASS
174	95	50	120	72.4	92208	PASS
175	174	5	9	7.4	6791	PASS
176	174	95	105	98.6	90917	PASS
177	176	5	10	6.5	5920	PASS

Scan 2775 (9.963 min): VV038687.D\data.ms
BFB205

m/z	Abundance
39.00	108.0
39.90	238.0
43.90	294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1114.0
37.00	5564.0
38.00	4885.0
39.00	2091.0
40.20	308.0
44.00	925.0
45.00	977.0
45.90	298.0
47.00	1241.0
48.00	876.0
49.00	4840.0
50.00	22008.0
51.00	6670.0
52.10	290.0
52.90	199.0
54.00	118.0
54.90	380.0
56.00	1856.0
57.00	3136.0
60.10	1130.0
61.00	6038.0
62.10	5664.0
63.10	5201.0
64.10	1099.0
65.00	1073.0
65.90	109.0
67.00	420.0
68.00	12183.0
69.00	12720.0
70.00	1011.0
72.10	626.0
73.00	5325.0
74.10	20984.0
75.00	59616.0
76.10	5340.0
77.00	864.0
77.70	528.0
78.90	5503.0
79.90	1727.0
80.90	4937.0
82.00	1182.0
86.00	233.0
87.00	5688.0
88.00	5307.0
90.80	492.0
92.10	3546.0
93.00	5241.0
94.00	14724.0
95.00	119872.0
96.00	7484.0
97.10	296.0
103.10	107.0
104.00	640.0
104.90	170.0
105.80	503.0
107.10	113.0
109.90	126.0
110.90	163.0
112.70	151.0
114.70	109.0
115.10	122.0
115.90	507.0
116.90	1061.0
117.90	548.0
118.90	817.0
127.90	340.0
129.00	265.0
129.90	380.0
131.00	219.0
134.90	277.0
136.90	204.0
141.00	1166.0
141.80	231.0
143.00	1768.0
143.80	146.0
145.00	788.0
145.90	262.0
147.70	247.0
152.80	113.0
154.90	164.0
156.90	218.0
159.00	125.0
160.90	202.0
171.10	344.0
172.00	1205.0
173.00	1523.0
174.00	83544.0
175.00	6452.0
176.00	82656.0
177.00	5378.0
178.00	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1179.0
37.00	6073.0
38.00	5058.0
39.00	2163.0
40.30	332.0
44.00	1000.0
45.00	1094.0
46.00	288.0
47.00	1506.0
48.00	904.0
49.00	5596.0
50.00	23832.0
51.00	7311.0
52.00	347.0
52.90	205.0
54.90	394.0
56.00	1962.0
57.00	3648.0
60.10	1285.0
61.00	6448.0
62.10	6292.0
63.10	5986.0
64.10	1057.0
65.00	1108.0
65.90	116.0
66.90	421.0
68.00	13279.0
69.10	14065.0
70.00	1053.0
72.00	754.0
73.00	5907.0
74.10	23392.0
75.00	65720.0
76.10	5784.0
77.00	915.0
77.80	512.0
78.90	6009.0
79.90	1834.0
80.90	5491.0
82.00	1306.0
82.80	111.0
86.00	268.0
87.00	6303.0
88.00	6012.0
90.80	545.0
92.10	3697.0
93.00	6035.0
94.00	15586.0
95.00	132096.0
96.10	8236.0
97.10	298.0
103.10	115.0
103.90	694.0
104.90	155.0
105.90	607.0
107.00	132.0
107.90	104.0
109.90	119.0
110.90	180.0
111.90	121.0
112.70	171.0
115.00	179.0
115.90	545.0
116.90	1052.0
117.90	631.0
118.90	954.0
127.90	381.0
129.00	395.0
129.90	455.0
130.90	259.0
135.00	358.0
136.90	226.0
141.00	1346.0
141.80	227.0
143.00	1928.0
143.80	149.0
145.00	885.0
145.90	257.0
147.70	259.0
149.90	102.0
152.80	166.0
154.90	203.0
157.00	279.0
159.00	145.0
160.90	226.0
171.00	355.0
172.00	1422.0
173.00	1577.0
174.00	95280.0
175.00	6957.0
176.00	94008.0
177.00	6162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

178.00

220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	1127.0
37.00	5929.0
38.00	5024.0
39.00	2081.0
40.20	303.0
43.20	127.0
44.00	1038.0
45.10	1061.0
46.00	255.0
47.00	1573.0
47.90	809.0
49.00	5508.0
50.00	23032.0
51.00	7417.0
52.00	340.0
53.10	181.0
54.90	392.0
56.00	1902.0
57.00	3681.0
60.10	1276.0
61.00	6444.0
62.10	6283.0
63.10	5878.0
64.00	1041.0
65.00	1040.0
65.80	134.0
67.00	374.0
68.00	13392.0
69.10	13863.0
70.10	1093.0
72.00	838.0
73.00	5786.0
74.10	23216.0
75.10	64712.0
76.10	5503.0
77.00	865.0
77.90	503.0
78.90	5825.0
79.90	1724.0
81.00	5582.0
81.90	1271.0
82.80	136.0
86.10	255.0
87.00	6043.0
88.00	5981.0
90.80	498.0
92.10	3508.0
93.00	6144.0
94.00	15363.0
95.00	130280.0
96.00	8415.0
97.10	250.0
103.10	109.0
103.90	697.0
104.90	144.0
105.90	715.0
107.00	143.0
110.90	192.0
111.90	120.0
112.70	144.0
114.90	193.0
115.80	514.0
116.90	972.0
117.90	636.0
118.90	1012.0
127.90	407.0
129.00	416.0
129.80	466.0
130.80	304.0
135.00	354.0
137.00	252.0
140.90	1368.0
141.80	137.0
143.00	1882.0
144.10	149.0
144.90	852.0
145.90	242.0
147.00	117.0
147.90	257.0
149.10	119.0
152.80	149.0
155.00	285.0
157.00	295.0
158.90	131.0
160.90	242.0
170.90	323.0
172.00	1436.0
172.90	1496.0
174.00	97800.0
175.00	6965.0
176.00	96088.0
177.00	6220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

178.10

250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205