




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024703.D
 Acq On : 16 Feb 2022 17:50
 Operator : SY/MD
 Sample : N1510-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M00

Manual IntegrationsAPPROVED

Quant Time: Feb 16 23:38:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/17/2022
 Supervised By :Mahesh Dadoda 02/18/2022

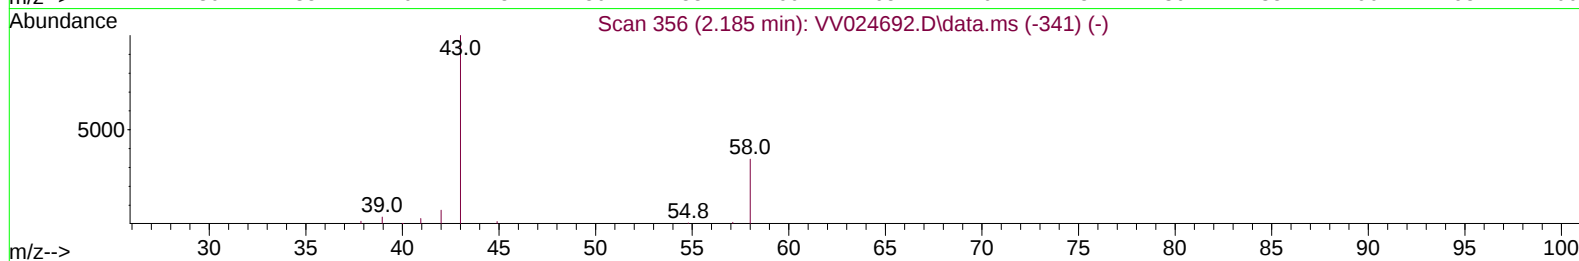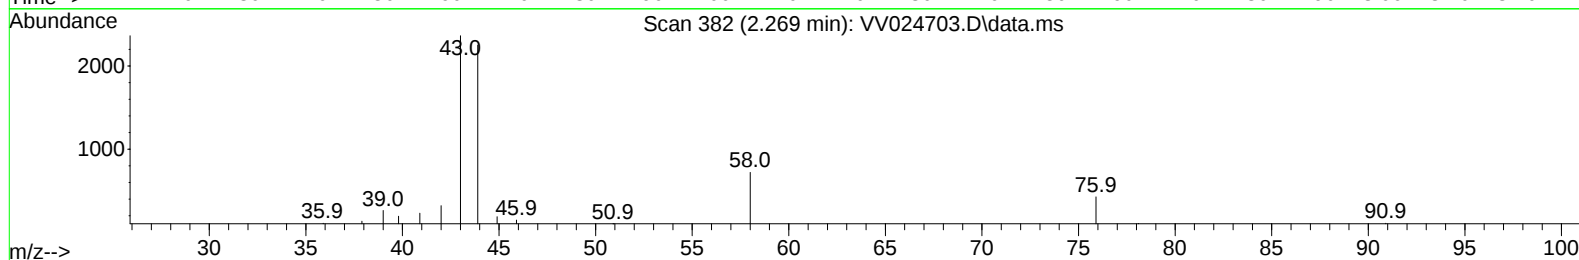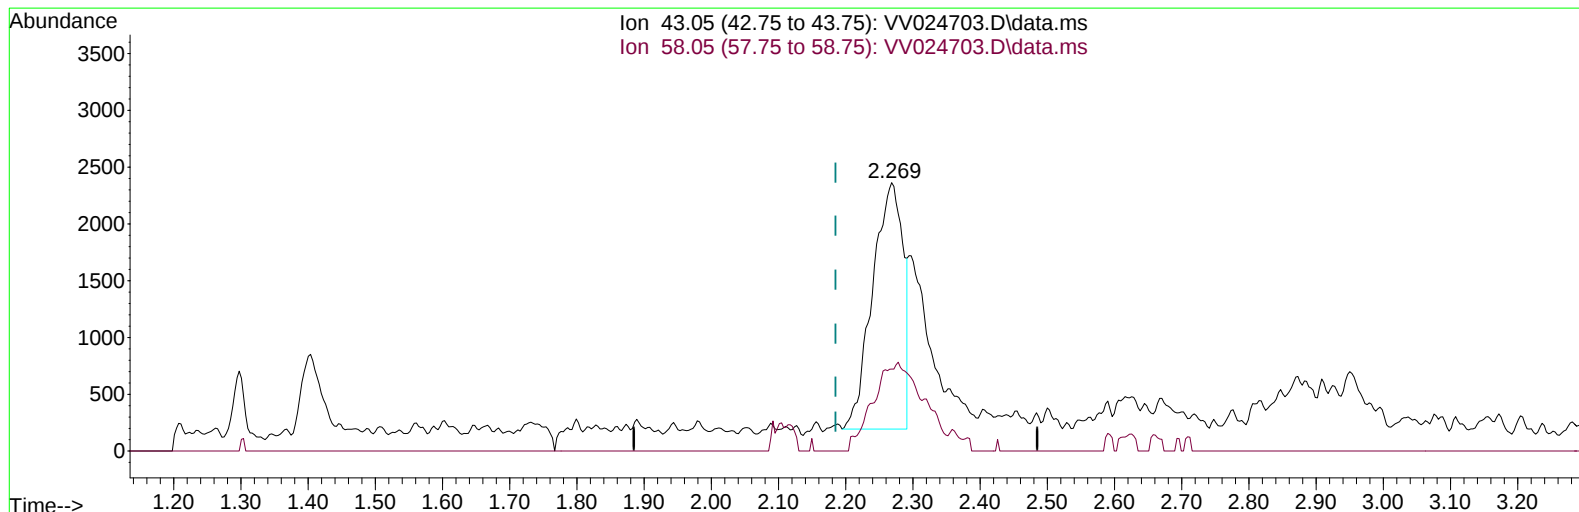

TIC: VV024703.D\data.ms

(13) Acetone (T)

2.269min (+ 0.083) 6.62 ug/L

response 6856

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	58.90#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024703.D
 Acq On : 16 Feb 2022 17:50
 Operator : SY/MD
 Sample : N1510-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M00

Manual IntegrationsAPPROVED

Quant Time: Feb 16 23:38:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/17/2022
 Supervised By :Mahesh Dadoda 02/18/2022

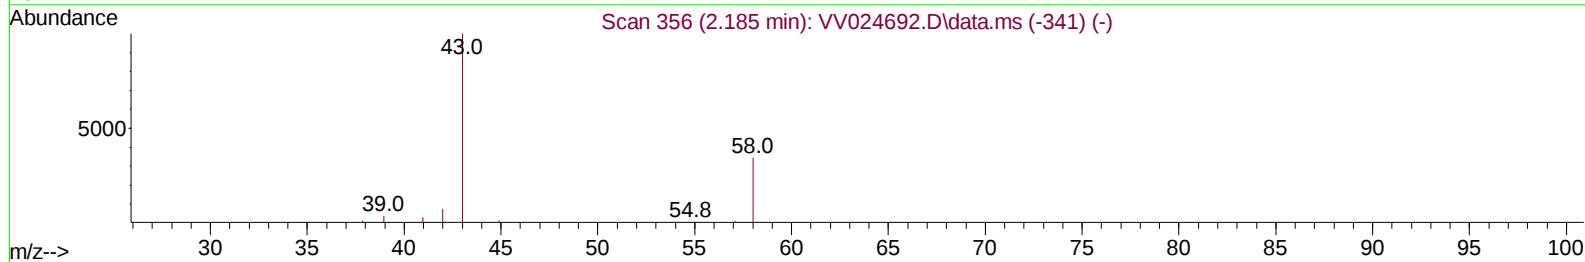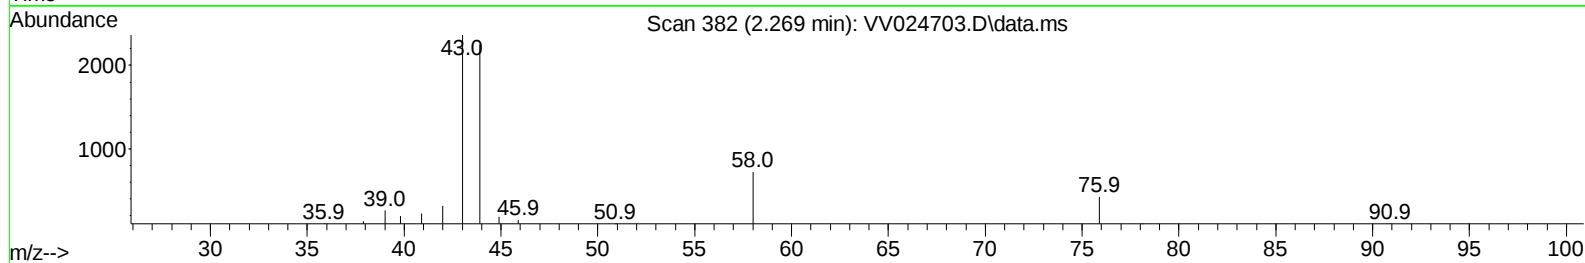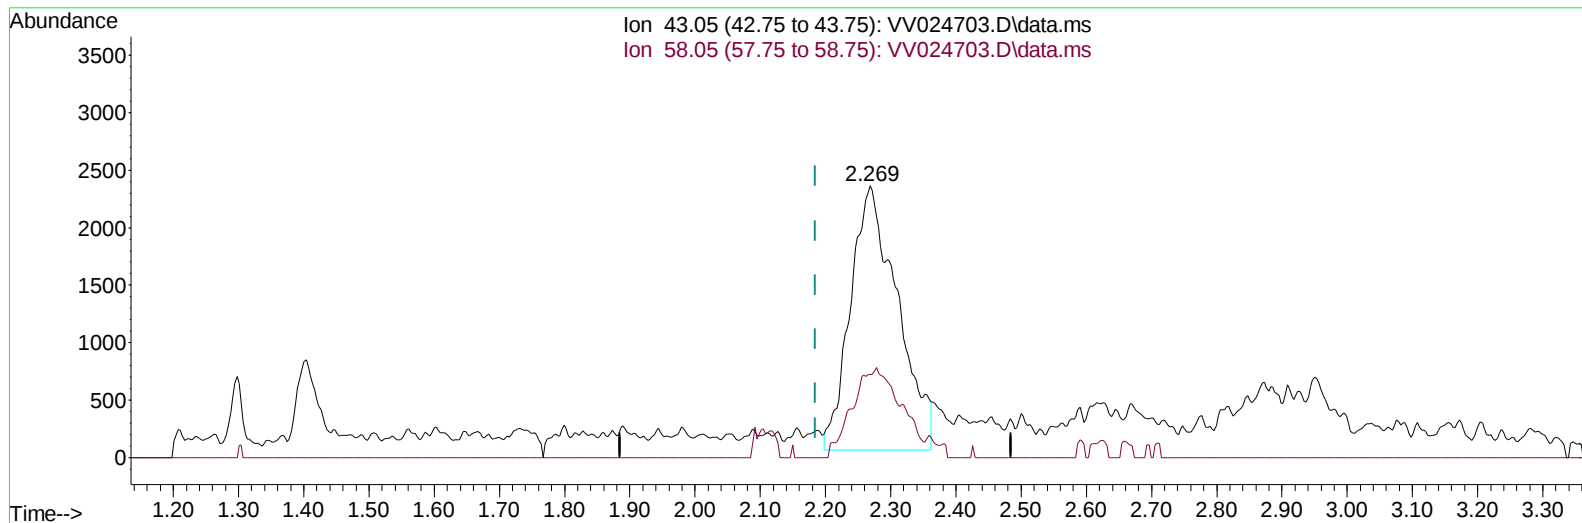

TIC: VV024703.D\data.ms

(13) Acetone (T)

2.269min (+ 0.083) 11.12 ug/L m

response 11512

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	35.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024703.D
 Acq On : 16 Feb 2022 17:50
 Operator : SY/MD
 Sample : N1510-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M00

Manual IntegrationsAPPROVED

Quant Time: Feb 16 23:38:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/17/2022
 Supervised By :Mahesh Dadoda 02/18/2022

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	94285	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	95484	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	46230	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.297	65	40611	5.138	ug/L	-0.01
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.800%	
7) Chloroethane-d5	1.558	69	39313	5.884	ug/L	-0.01
Spiked Amount	5.000	Range 65 - 130	Recovery	=	117.600%	
11) 1,1-Dichloroethene-d2	2.098	63	61992	3.586	ug/L	-0.02
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.800%	
20) 2-Butanone-d5	3.969	46	77602	59.148	ug/L	0.08
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.300%	
24) Chloroform-d	4.346	84	85807	6.169	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	123.400%	
26) 1,2-Dichloroethane-d4	5.034	65	41184	6.525	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	130.600%#	
32) Benzene-d6	5.043	84	169567	6.259	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	125.200%#	
36) 1,2-Dichloropropane-d6	6.069	67	52225	6.198	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	124.000%	
41) Toluene-d8	7.313	98	145204	5.747	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	115.000%	
43) trans-1,3-Dichloroprop...	7.625	79	16747	4.921	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.400%	
46) 2-Hexanone-d5	8.098	63	57470	47.938	ug/L	0.01
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.880%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	30097	5.999	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	120.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	49124	6.592	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	131.800%#	
Target Compounds						
13) Acetone	2.269	43	11512m	11.119	ug/L	
14) Carbon disulfide	2.285	76	1776	0.057	ug/L #	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024703.D
Acq On : 16 Feb 2022 17:50
Operator : SY/MD
Sample : N1510-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M00

Manual IntegrationsAPPROVED

Quant Time: Feb 16 23:38:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 23:36:08 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/17/2022
Supervised By :Mahesh Dadoda 02/18/2022

