

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021622\
 Data File : VW024696.D
 Acq On : 16 Feb 2022 15:07
 Operator : SY/MD
 Sample : N1475-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Feb 16 23:37:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	168403	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	170101	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	82393	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	68444	4.849	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.571	69	57587	4.825	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.600%
11) 1,1-Dichloroethene-d2	2.111	63	98375	3.186	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.800%
20) 2-Butanone-d5	3.896	46	100334	42.816	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.640%
24) Chloroform-d	4.349	84	107299	4.319	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	5.031	65	52034	4.616	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	5.047	84	229783	4.761	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%
36) 1,2-Dichloropropane-d6	6.066	67	67334	4.486	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.800%
41) Toluene-d8	7.313	98	201485	4.476	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	7.622	79	22572	3.724	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.088	63	86416	40.463	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.920%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37481	4.194	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	63541	4.784	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds					Qvalue	
25) Chloroform	4.375	83	3563	0.115	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024696.D
Acq On : 16 Feb 2022 15:07
Operator : SY/MD
Sample : N1475-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Feb 16 23:37:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 23:36:08 2022
Response via : Initial Calibration

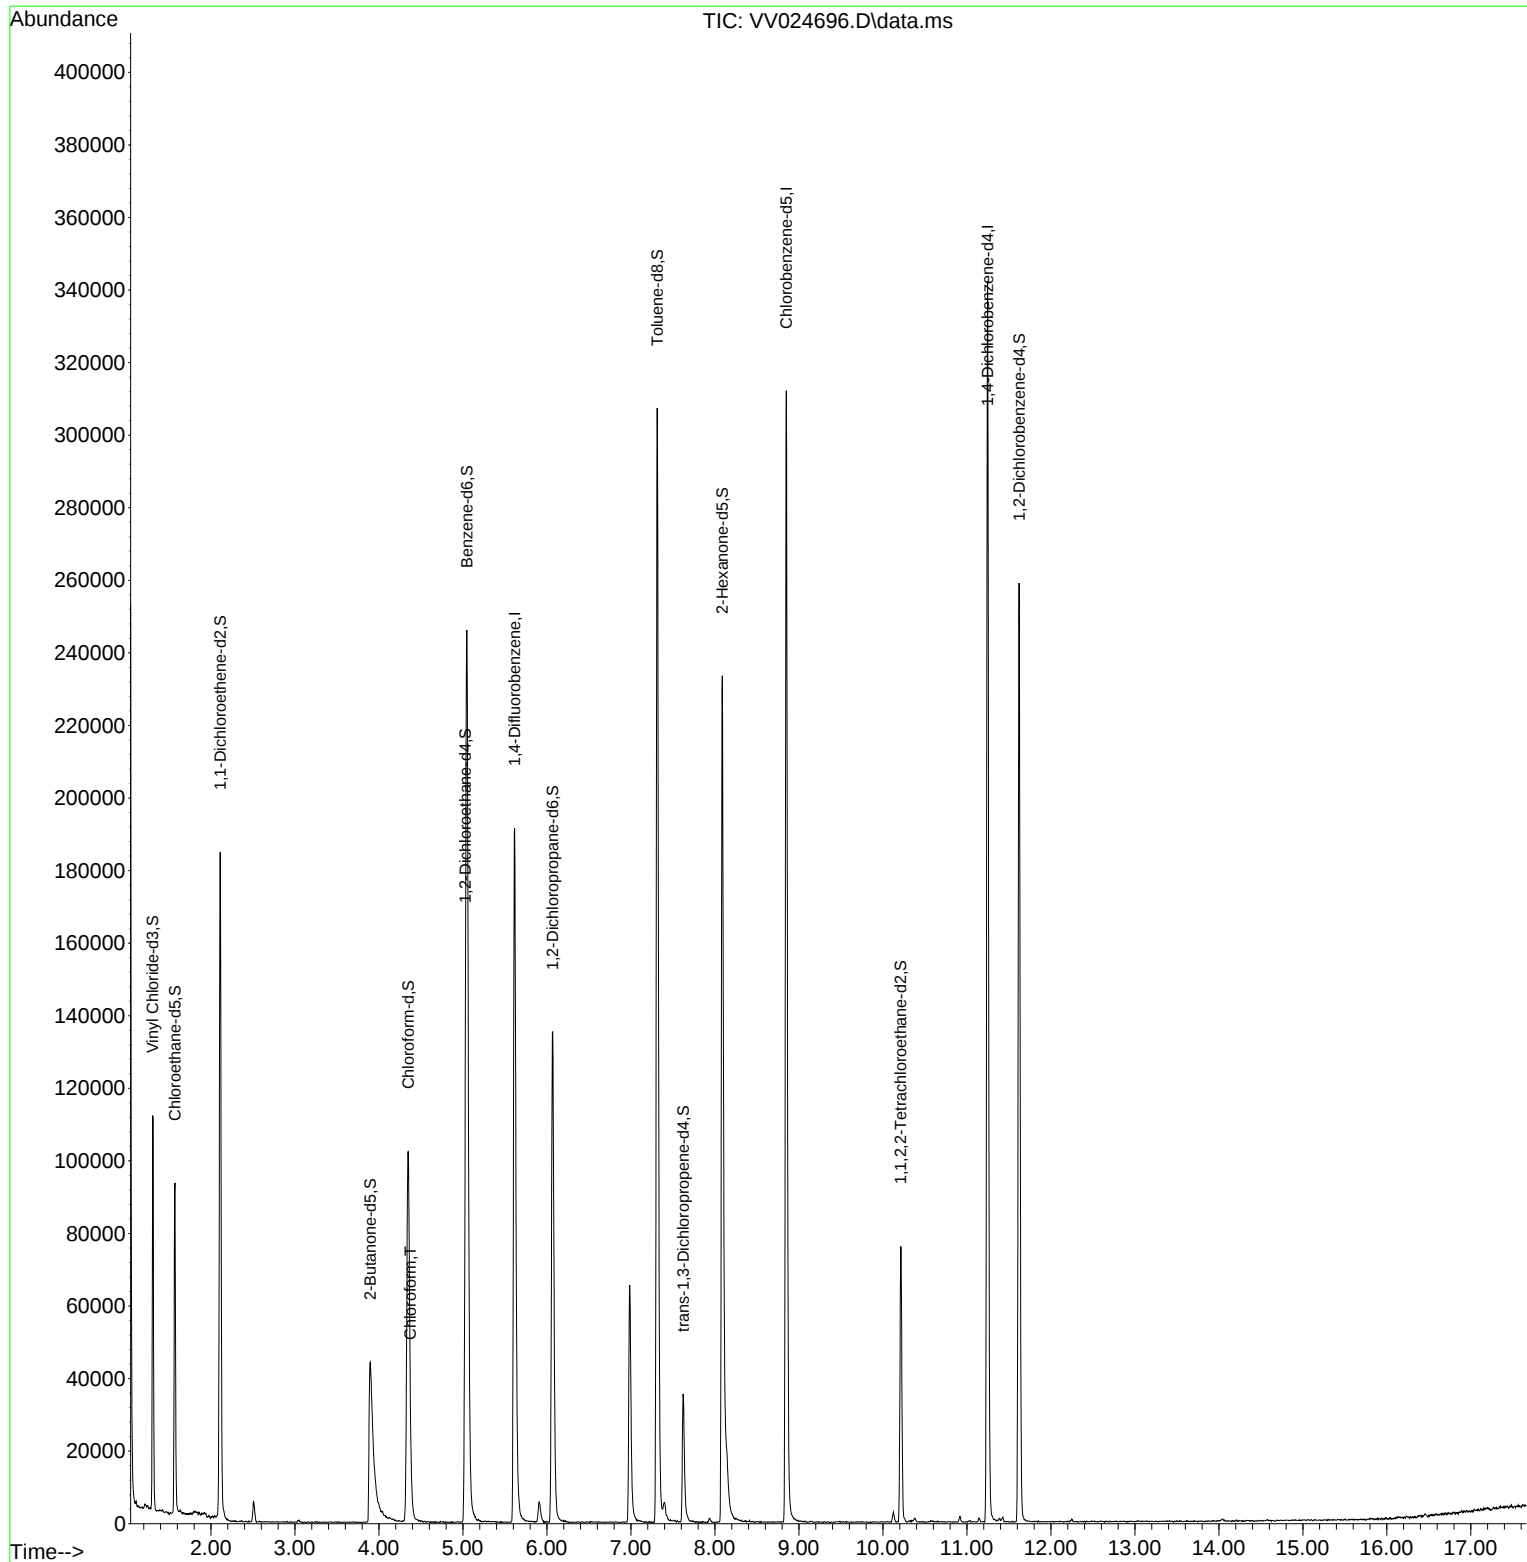

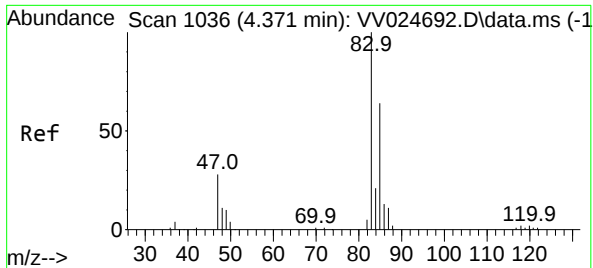

#25
 Chloroform
 Concen: 0.115 ug/L
 RT: 4.375 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VV024696.D
 Acq: 16 Feb 2022 15:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 83 Resp: 3563
 Ion Ratio Lower Upper
 83 100
 85 66.1 45.2 84.0

