

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021622\
 Data File : VW024699.D
 Acq On : 16 Feb 2022 16:17
 Operator : SY/MD
 Sample : N1480-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY2

Quant Time: Feb 16 23:37:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	110818	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	109816	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55106	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41794	4.499	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.000%	
7) Chloroethane-d5	1.571	69	45140	5.748	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	115.000%	
11) 1,1-Dichloroethene-d2	2.111	63	66616	3.279	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.600%	
20) 2-Butanone-d5	3.896	46	101571	65.867	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	131.740%#	
24) Chloroform-d	4.352	84	94259	5.766	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	115.400%	
26) 1,2-Dichloroethane-d4	5.034	65	44724	6.029	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	120.600%	
32) Benzene-d6	5.053	84	186871	5.997	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	120.000%	
36) 1,2-Dichloropropane-d6	6.069	67	59178	6.107	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	122.200%	
41) Toluene-d8	7.317	98	159890	5.502	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.000%	
43) trans-1,3-Dichloroprop...	7.625	79	18615	4.756	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.200%	
46) 2-Hexanone-d5	8.088	63	82669	59.957	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	119.920%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	37340	6.471	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	129.400%#	
66) 1,2-Dichlorobenzene-d4	11.622	152	54697	6.157	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	123.200%#	
Target Compounds						Qvalue
51) Chlorobenzene	8.886	112	5116	0.179	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024699.D
Acq On : 16 Feb 2022 16:17
Operator : SY/MD
Sample : N1480-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY2

Quant Time: Feb 16 23:37:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 23:36:08 2022
Response via : Initial Calibration

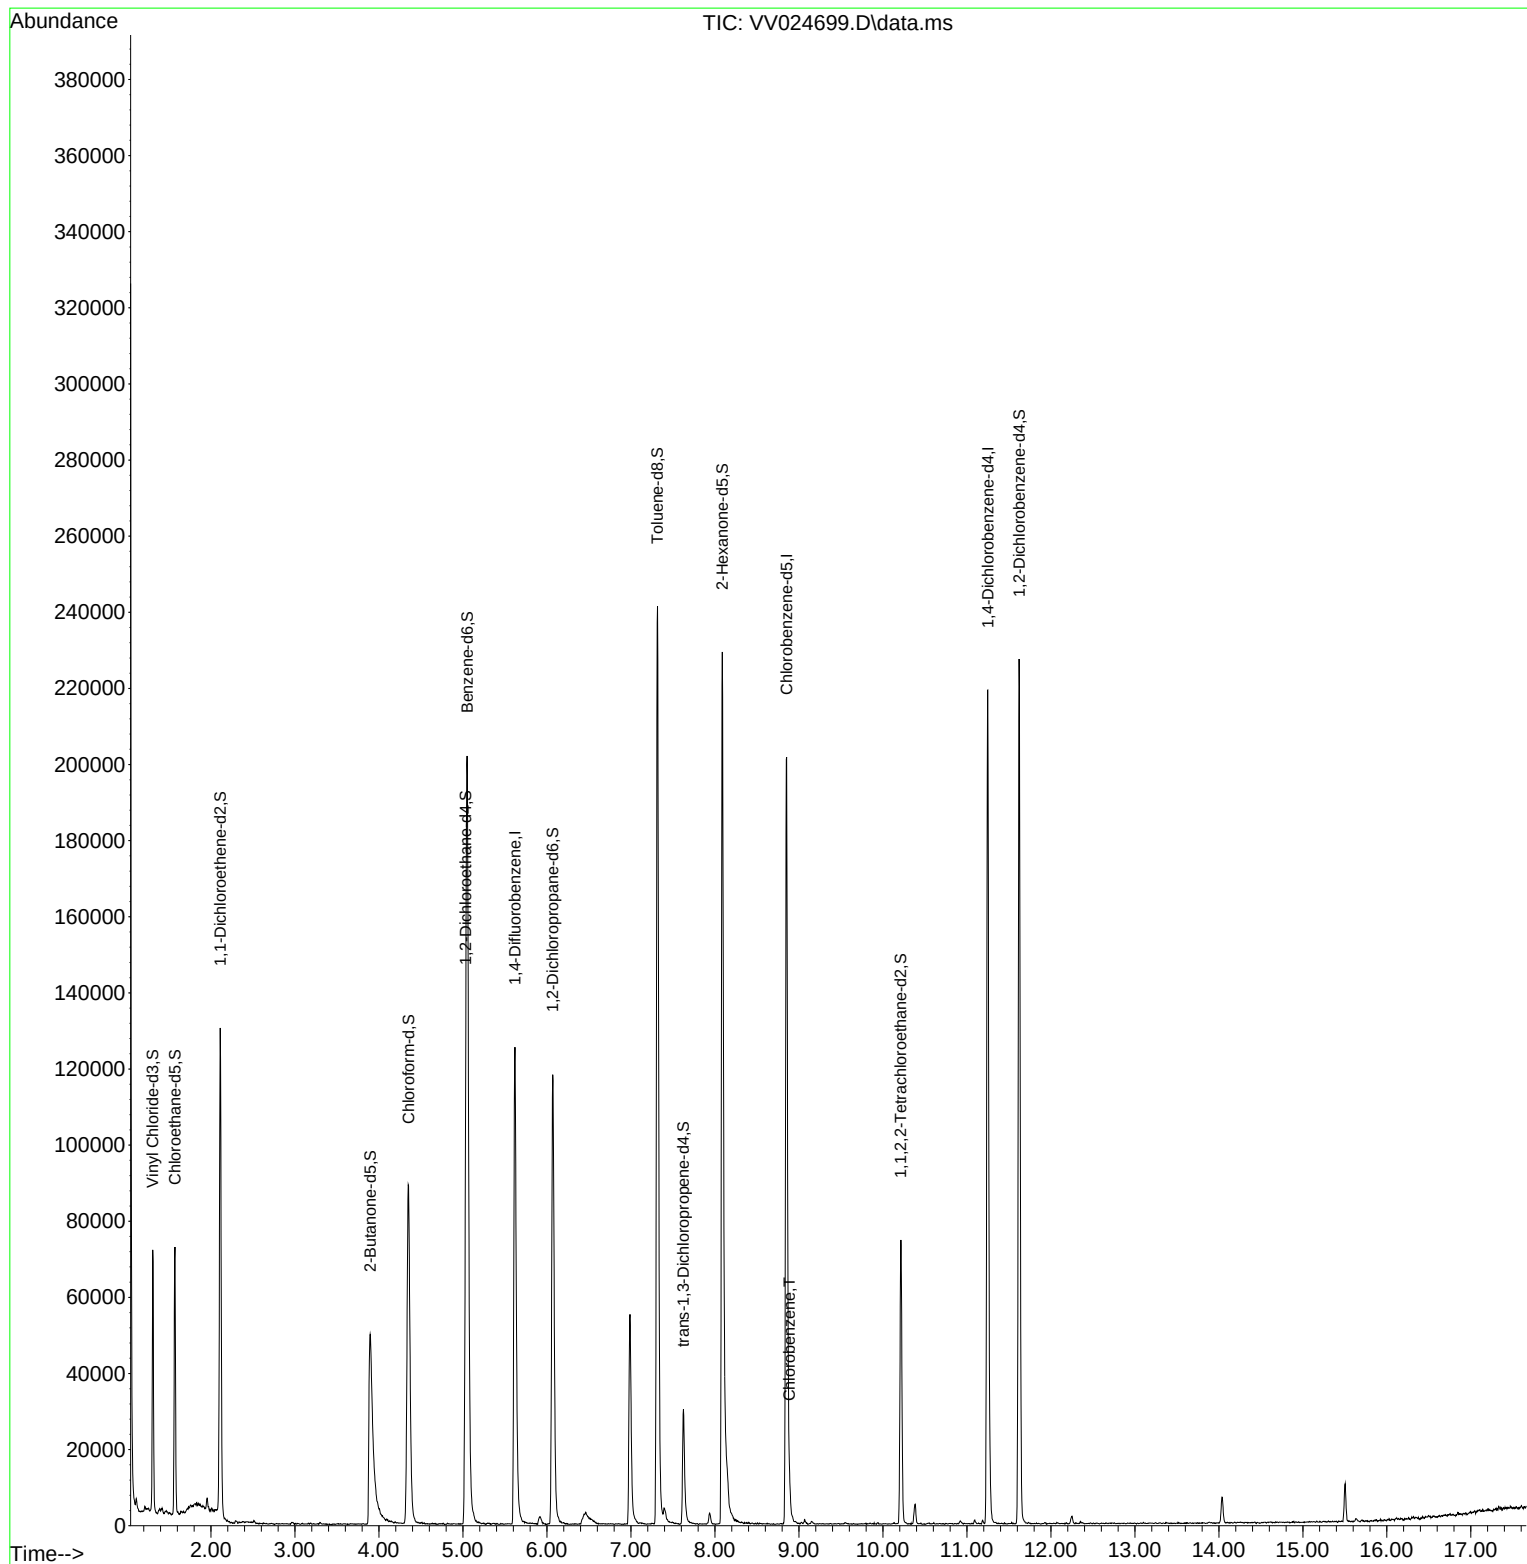

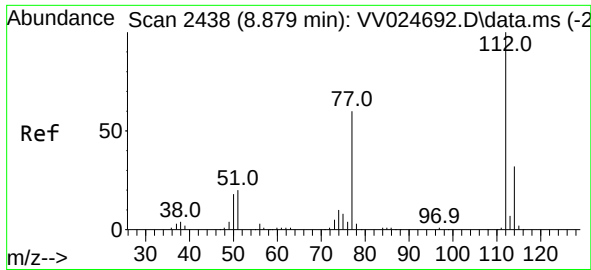

#51
Chlorobenzene
Concen: 0.179 ug/L
RT: 8.886 min Scan# 24
Delta R.T. 0.007 min
Lab File: VV024699.D
Acq: 16 Feb 2022 16:17

Instrument :
MSVOA_V
ClientSampleId :
GBCY2

Tgt Ion:112	Resp:	5116
Ion Ratio	Lower	Upper
112	100	
114	34.5	23.3 43.3
77	64.1	43.3 64.9

