

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021622\
 Data File : VW024700.D
 Acq On : 16 Feb 2022 16:40
 Operator : SY/MD
 Sample : N1480-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY3

Quant Time: Feb 16 23:38:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	110164	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	111579	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56319	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42604	4.614	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.200%
7) Chloroethane-d5	1.571	69	43430	5.563	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.200%
11) 1,1-Dichloroethene-d2	2.111	63	67602	3.347	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.000%
20) 2-Butanone-d5	3.896	46	98523	64.270	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.540%
24) Chloroform-d	4.352	84	93794	5.771	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.400%
26) 1,2-Dichloroethane-d4	5.034	65	45893	6.223	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.400%
32) Benzene-d6	5.053	84	186067	5.877	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.600%
36) 1,2-Dichloropropane-d6	6.069	67	59137	6.006	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	120.200%
41) Toluene-d8	7.317	98	160672	5.441	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%
43) trans-1,3-Dichloroprop...	7.625	79	19027	4.785	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.600%
46) 2-Hexanone-d5	8.088	63	83070	59.296	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.600%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36492	6.224	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.400%#
66) 1,2-Dichlorobenzene-d4	11.622	152	54025	5.951	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.000%
Target Compounds						Qvalue
51) Chlorobenzene	8.886	112	9364	0.322	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024700.D
Acq On : 16 Feb 2022 16:40
Operator : SY/MD
Sample : N1480-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCY3

Quant Time: Feb 16 23:38:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 23:36:08 2022
Response via : Initial Calibration

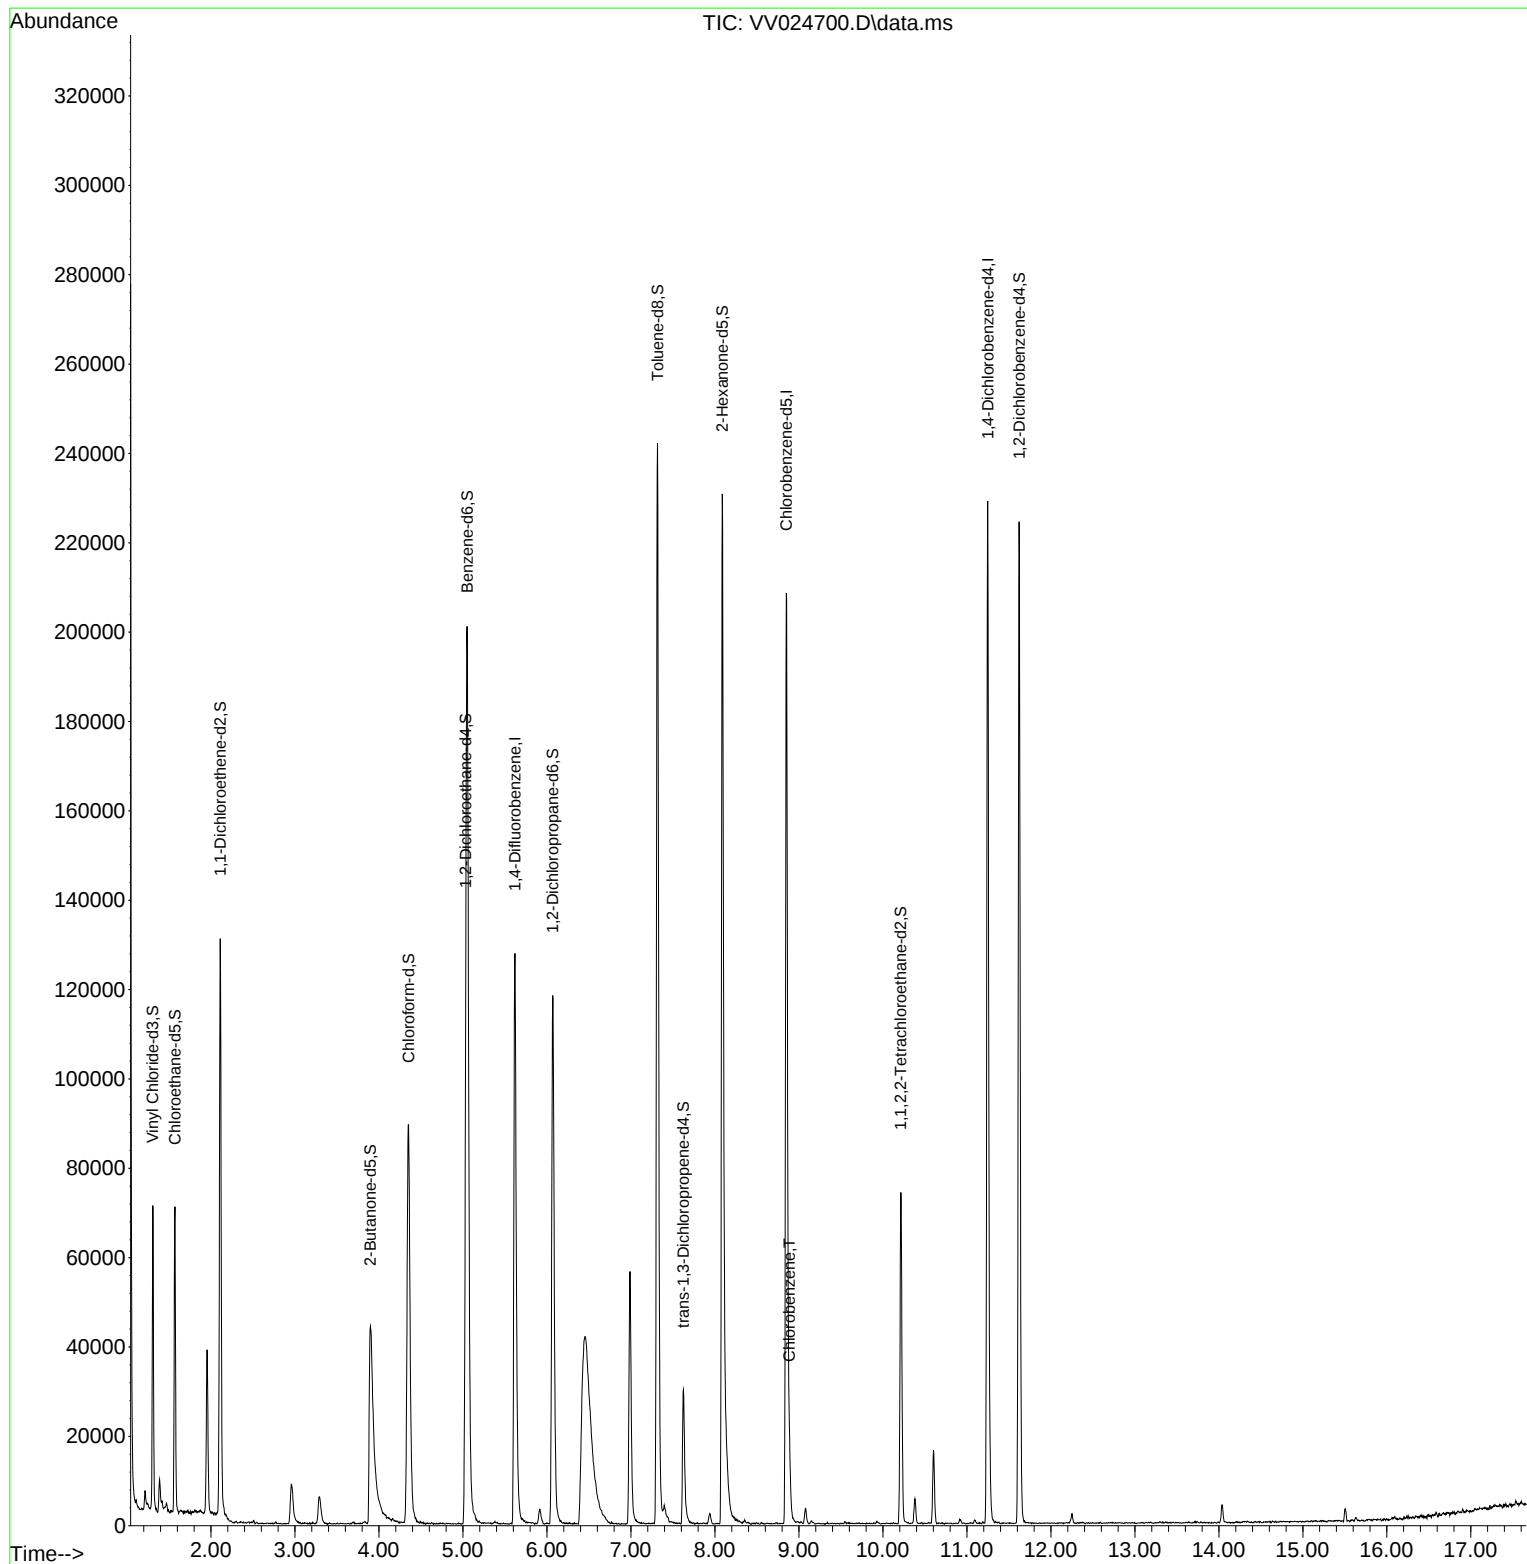

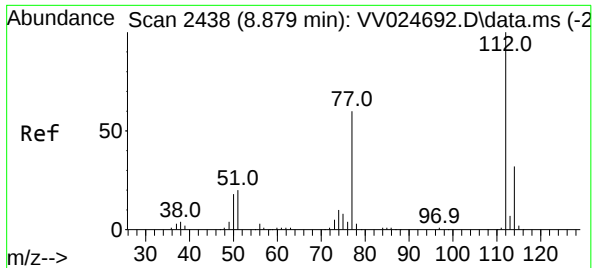

#51
 Chlorobenzene
 Concen: 0.322 ug/L
 RT: 8.886 min Scan# 24
 Delta R.T. 0.006 min
 Lab File: VV024700.D
 Acq: 16 Feb 2022 16:40

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCY3

Tgt Ion:112 Resp: 9364
 Ion Ratio Lower Upper
 112 100
 114 34.1 23.3 43.3
 77 55.4 43.3 64.9

