

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021622\
 Data File : VW024707.D
 Acq On : 16 Feb 2022 19:23
 Operator : SY/MD
 Sample : N1510-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M19

Quant Time: Feb 16 23:39:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 16 23:36:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	103728	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	102681	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51116	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42237	4.858	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.200%
7) Chloroethane-d5	1.568	69	43970	5.982	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	119.600%
11) 1,1-Dichloroethene-d2	2.108	63	65507	3.444	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	3.912	46	67616	46.845	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.680%
24) Chloroform-d	4.352	84	91195	5.959	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	119.200%
26) 1,2-Dichloroethane-d4	5.034	65	43248	6.228	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.600%
32) Benzene-d6	5.050	84	174706	5.997	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	120.000%
36) 1,2-Dichloropropane-d6	6.069	67	54875	6.056	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	121.200%
41) Toluene-d8	7.313	98	148848	5.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%
43) trans-1,3-Dichloroprop...	7.625	79	17307	4.730	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%
46) 2-Hexanone-d5	8.091	63	74001	57.400	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.800%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36454	6.757	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	135.200%#
66) 1,2-Dichlorobenzene-d4	11.622	152	50959	6.184	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	123.600%#
Target Compounds						
					Qvalue	
13) Acetone	2.204	43	6797	5.967	ug/L	95
14) Carbon disulfide	2.294	76	6383	0.187	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024707.D
Acq On : 16 Feb 2022 19:23
Operator : SY/MD
Sample : N1510-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M19

Quant Time: Feb 16 23:39:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 16 23:36:08 2022
Response via : Initial Calibration

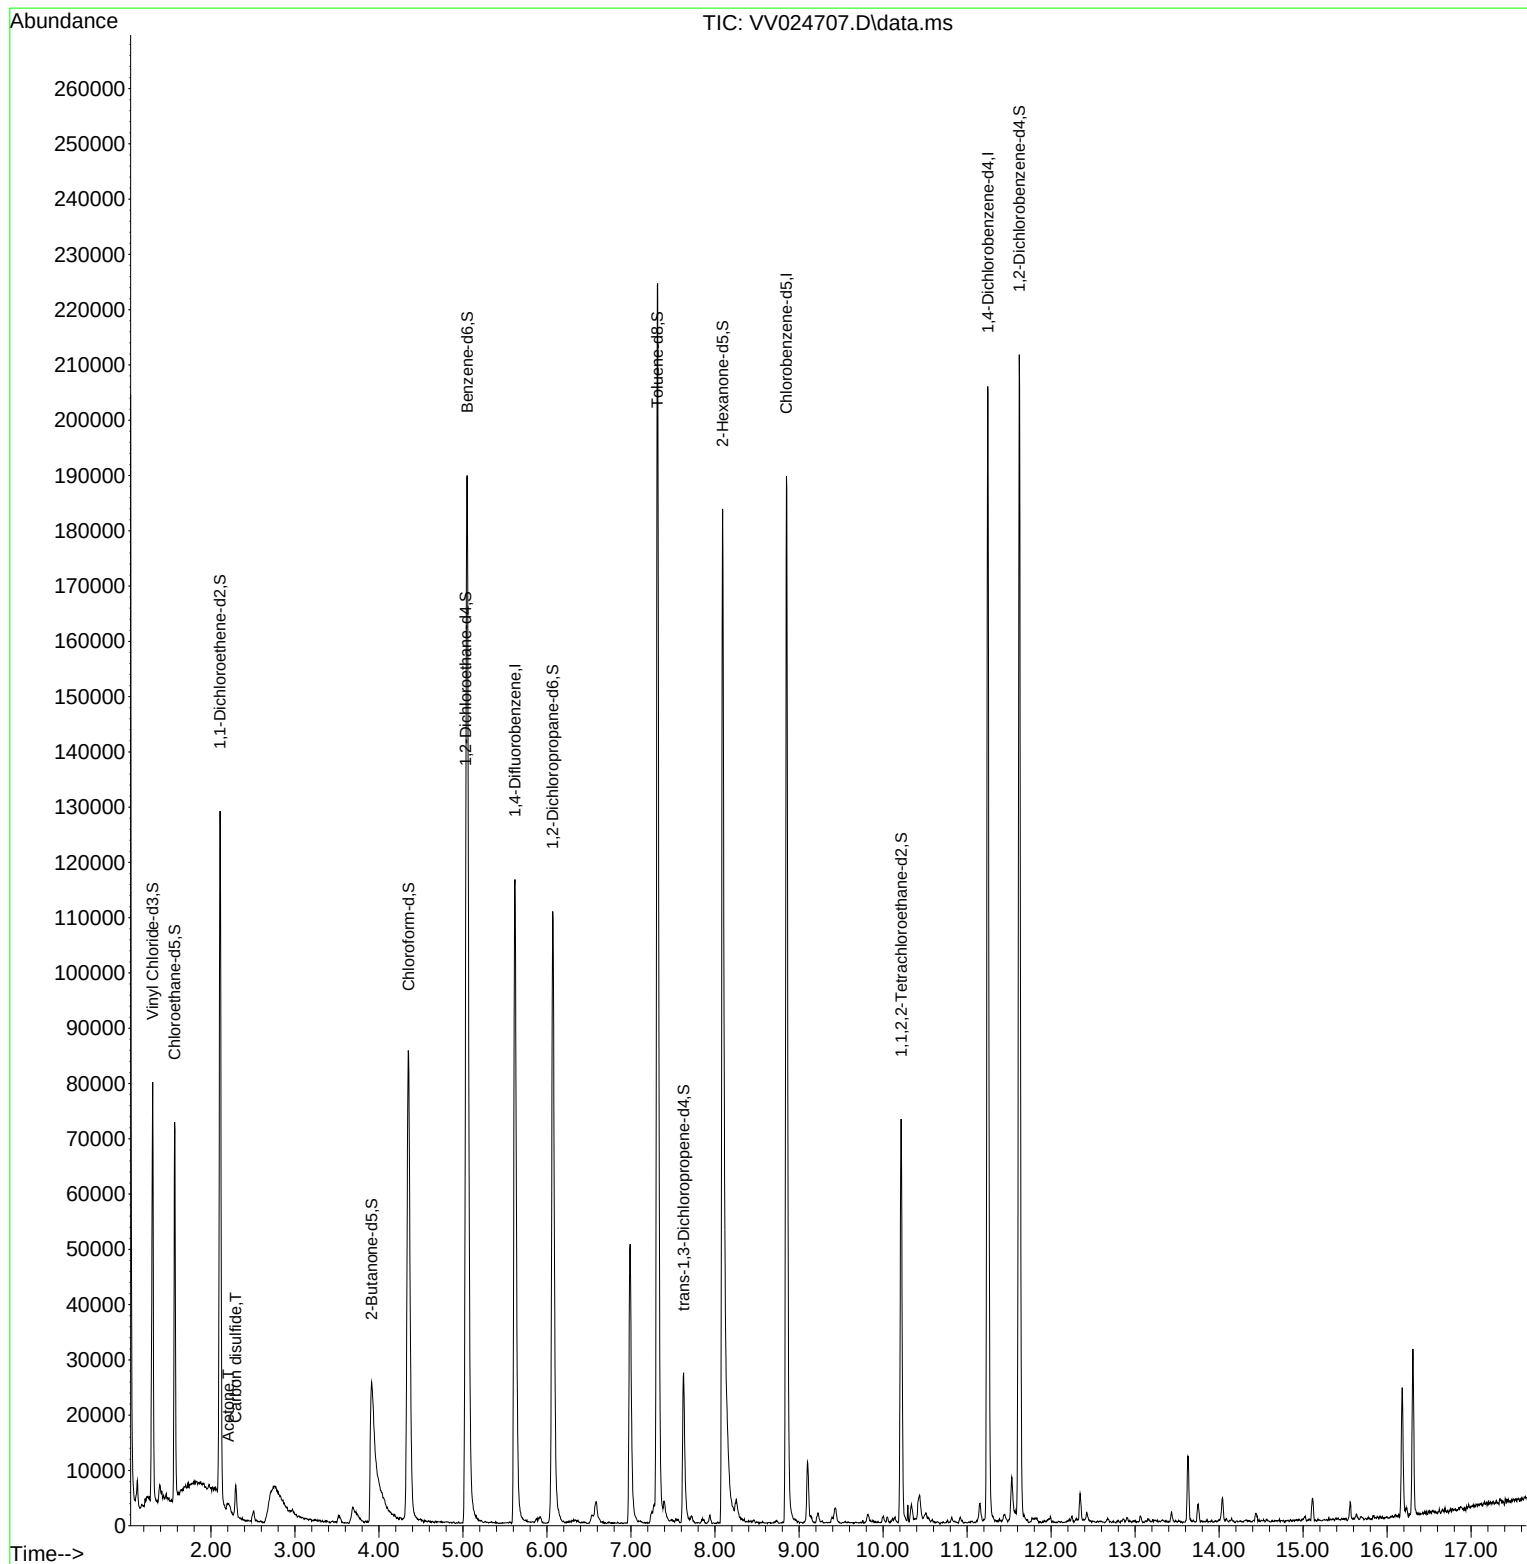

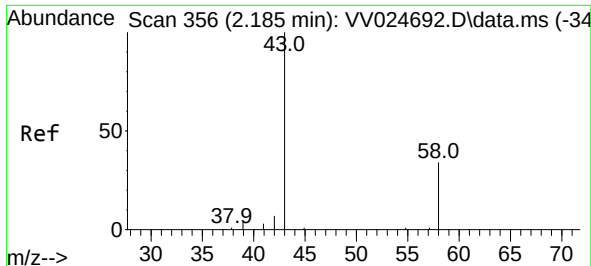

#13

Acetone

Concen: 5.967 ug/L

RT: 2.204 min Scan# 3

Delta R.T. 0.019 min

Lab File: VV024707.D

Acq: 16 Feb 2022 19:23

Instrument :

MSVOA_V

ClientSampleId :





F4M19

Tgt Ion: 43 Resp: 6797

Ion Ratio Lower Upper

43 100

58 18.3 0.0 41.4

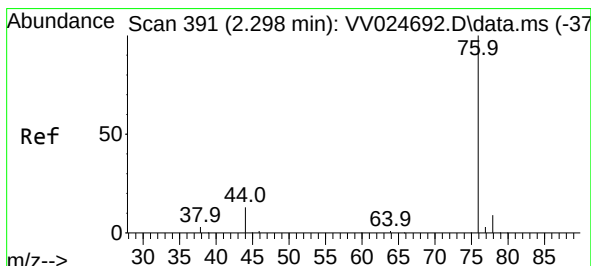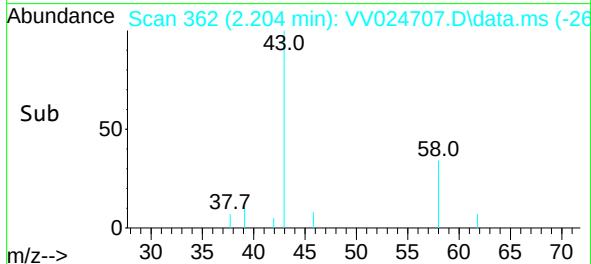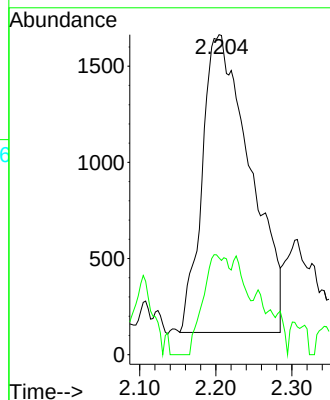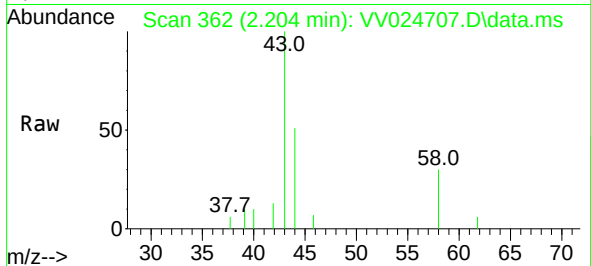

#14

Carbon disulfide

Concen: 0.187 ug/L

RT: 2.294 min Scan# 390

Delta R.T. -0.003 min

Lab File: VV024707.D

Acq: 16 Feb 2022 19:23

Tgt Ion: 76 Resp: 6383

Ion Ratio Lower Upper

76 100

78 10.2 7.5 11.3

