

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024693.D
 Acq On : 16 Feb 2022 13:37
 Operator : SY/MD
 Sample : VV0216WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK306

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	97	rVB	69639	71586	14.16%	1.776%
2	1.571	157	165	176	rBV	69222	78459	15.52%	1.946%
3	2.111	321	333	352	rVB	130680	190304	37.64%	4.721%
4	3.895	879	888	930	rBV2	40917	153356	30.33%	3.804%
5	4.349	1012	1029	1054	rBV	88161	224787	44.46%	5.576%
6	5.046	1230	1246	1284	rBV2	201406	505555	100.00%	12.542%
7	5.616	1411	1423	1447	rBV	141572	285787	56.53%	7.090%
8	5.911	1502	1515	1531	rVB5	4646	10637	2.10%	0.264%
9	6.069	1550	1564	1591	rBV2	116696	241764	47.82%	5.998%
10	6.985	1838	1849	1868	rBV	55629	103471	20.47%	2.567%
11	7.313	1939	1951	1970	rBV	241337	424431	83.95%	10.529%
12	7.622	2038	2047	2067	rBV	31002	55884	11.05%	1.386%
13	8.088	2182	2192	2236	rBV	217035	435509	86.14%	10.804%
14	8.850	2419	2429	2449	rBV	229942	375837	74.34%	9.324%
15	10.213	2839	2853	2870	rBV	69758	109837	21.73%	2.725%
16	11.249	3164	3175	3196	rBV	249314	390868	77.31%	9.697%
17	11.622	3280	3291	3311	rBV	222878	352051	69.64%	8.734%
18	12.249	3474	3486	3497	rBV	7613	11816	2.34%	0.293%
19	14.040	4033	4043	4056	rVB	5292	9063	1.79%	0.225%




Sum of corrected areas: 4031002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024693.D
Acq On : 16 Feb 2022 13:37
Operator : SY/MD
Sample : VV0216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

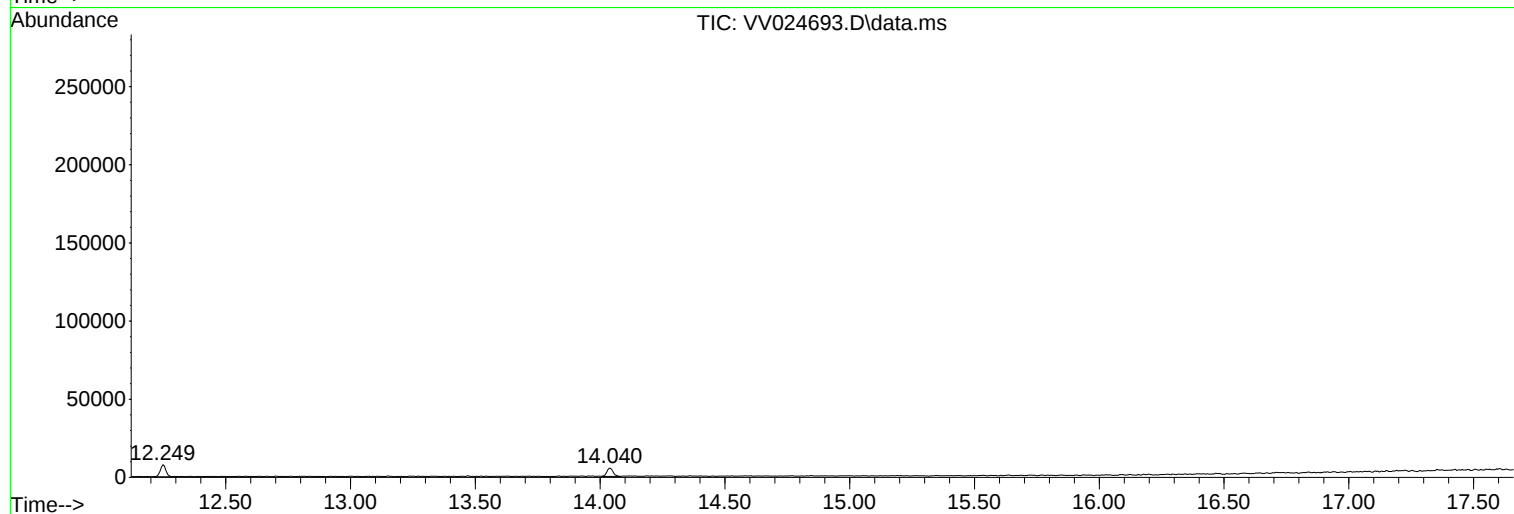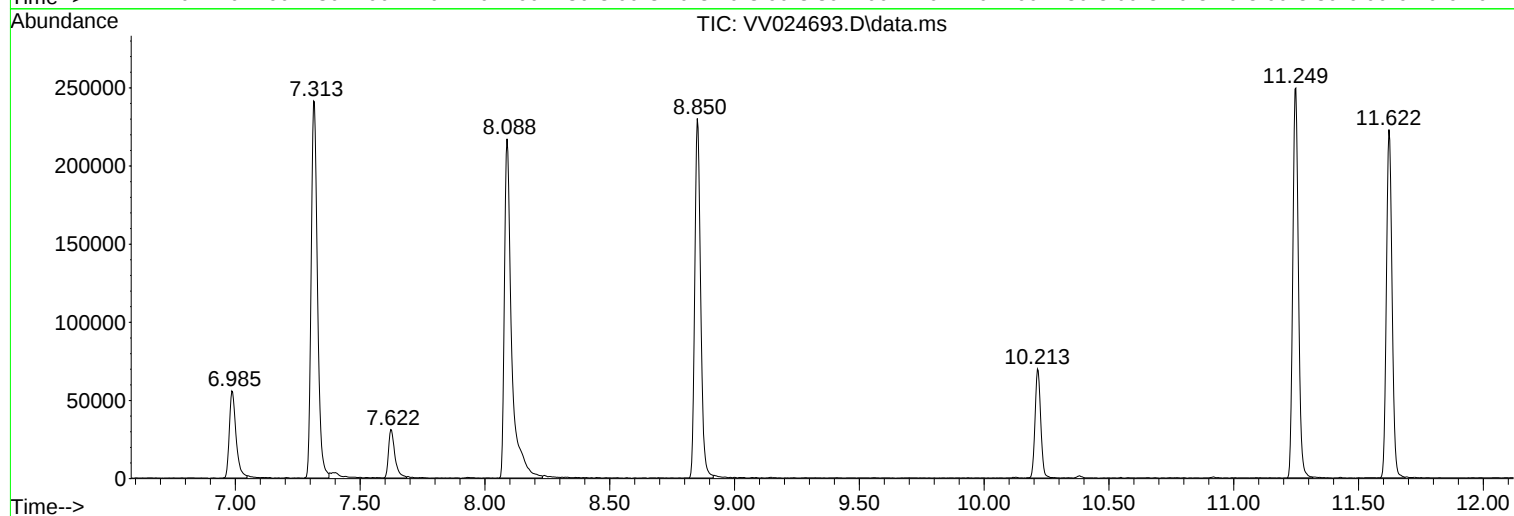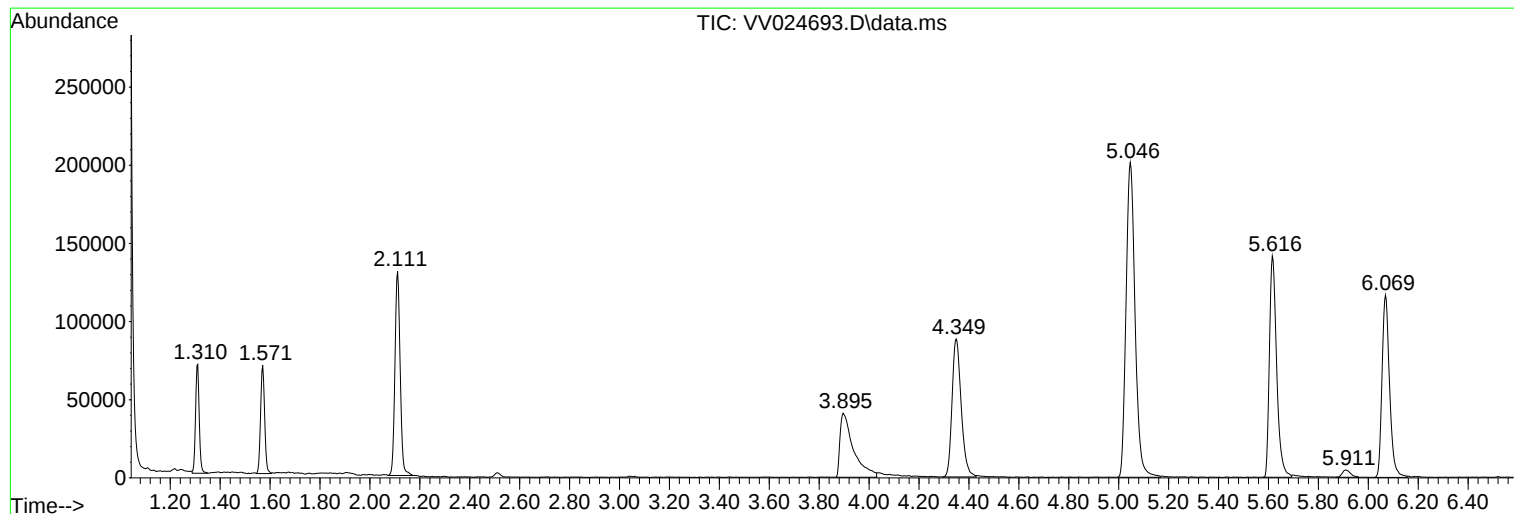

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024693.D
Acq On : 16 Feb 2022 13:37
Operator : SY/MD
Sample : VV0216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024693.D
Acq On : 16 Feb 2022 13:37
Operator : SY/MD
Sample : VV0216WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK306

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc