

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024694.D
 Acq On : 16 Feb 2022 14:15
 Operator : SY/MD
 Sample : N1475-15DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M90DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	59836	63423	5.90%	1.261%
2	1.568	156	164	177	rBV	62529	71626	6.66%	1.425%
3	2.101	319	330	350	rVB	117000	171416	15.95%	3.409%
4	3.892	877	887	914	rBV2	40068	135680	12.62%	2.699%
5	4.342	1012	1027	1055	rBV	80401	211735	19.70%	4.211%
6	5.040	1229	1244	1273	rBV2	184730	459847	42.78%	9.146%
7	5.612	1409	1422	1448	rBV	169093	342201	31.83%	6.806%
8	6.066	1550	1563	1587	rBV	105500	214288	19.93%	4.262%
9	6.985	1838	1849	1876	rBV	49821	94796	8.82%	1.885%
10	7.313	1937	1951	1962	rBV	218693	386077	35.91%	7.679%
11	7.381	1962	1972	1997	rVB	624434	1074994	100.00%	21.380%
12	7.622	2038	2047	2065	rBV2	28107	48636	4.52%	0.967%
13	8.088	2181	2192	2229	rBV	165007	393067	36.56%	7.818%
14	8.850	2417	2429	2452	rBV	270715	445433	41.44%	8.859%
15	10.214	2842	2853	2874	rVB	60710	98656	9.18%	1.962%
16	11.246	3163	3174	3197	rBV	308657	468453	43.58%	9.317%
17	11.622	3277	3291	3312	rBV	206733	320486	29.81%	6.374%
18	12.249	3475	3486	3498	rBV2	6962	11151	1.04%	0.222%
19	14.037	4032	4042	4056	rBV	10083	15961	1.48%	0.317%




Sum of corrected areas: 5027926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024694.D
Acq On : 16 Feb 2022 14:15
Operator : SY/MD
Sample : N1475-15DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

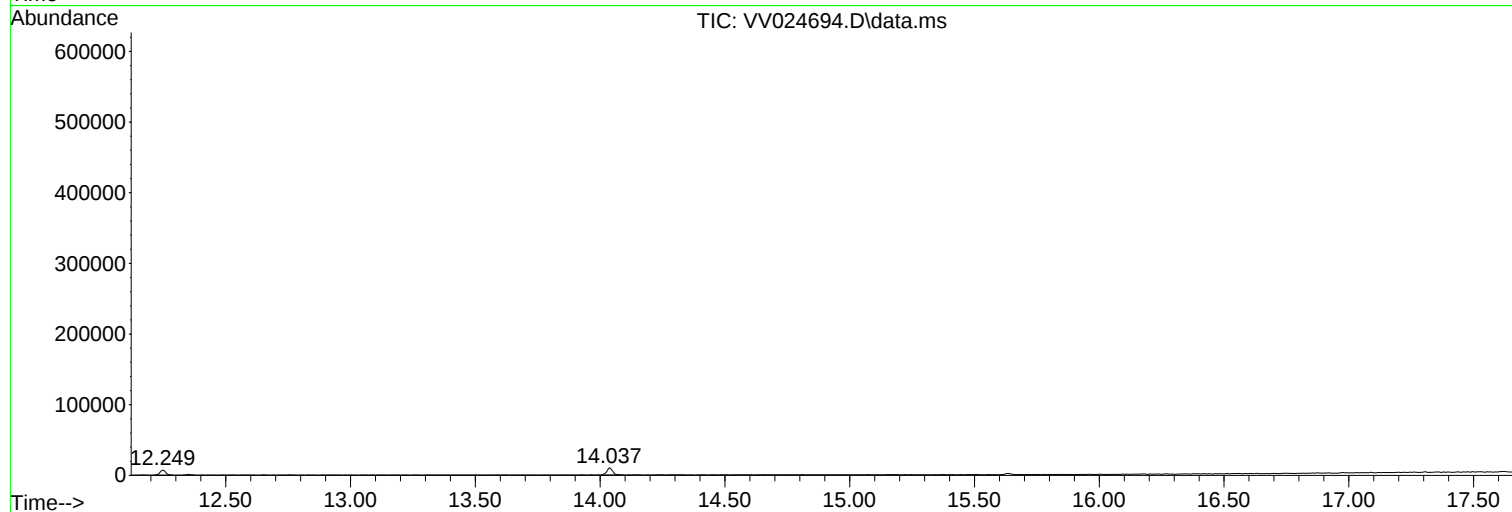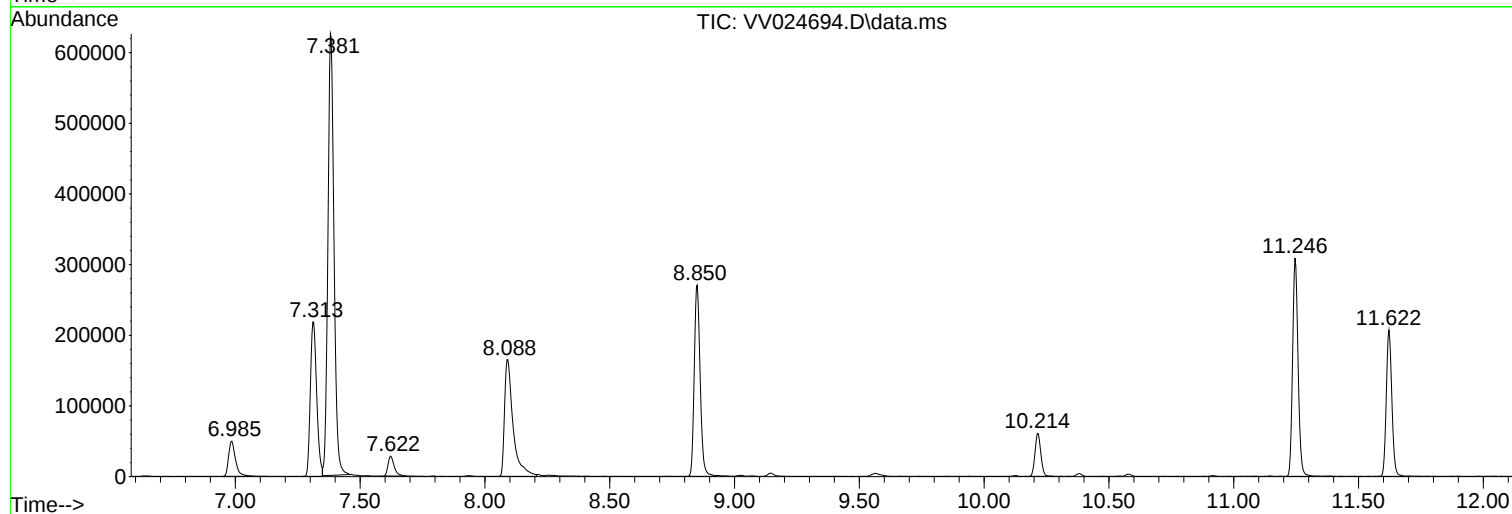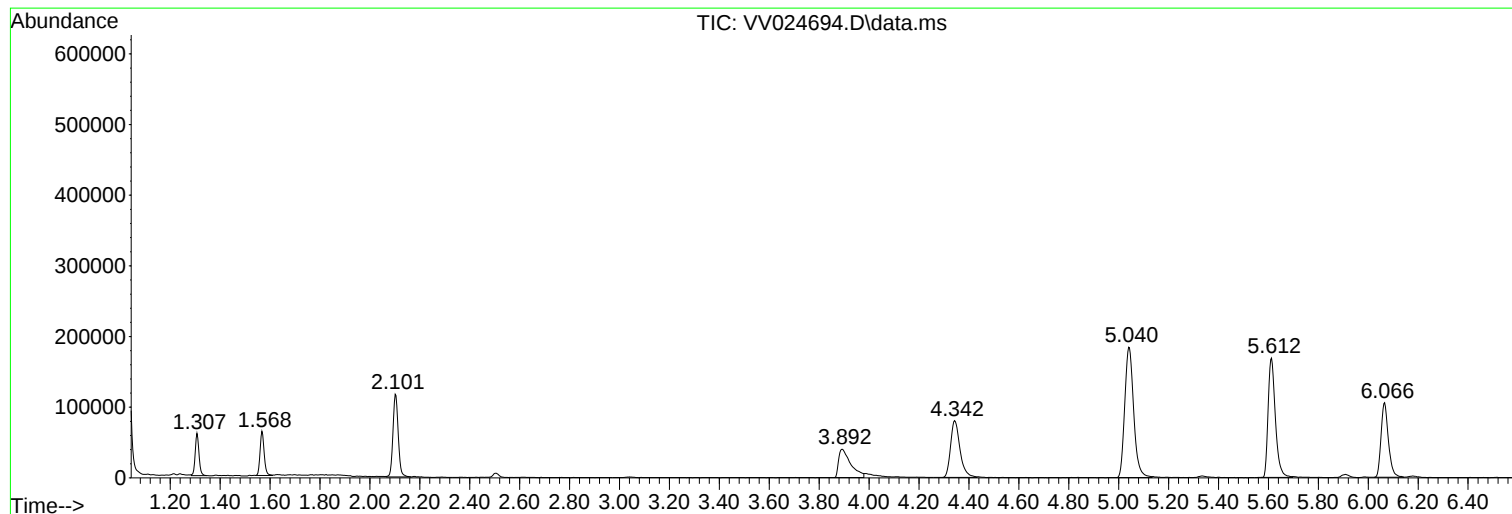

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024694.D
Acq On : 16 Feb 2022 14:15
Operator : SY/MD
Sample : N1475-15DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024694.D
Acq On : 16 Feb 2022 14:15
Operator : SY/MD
Sample : N1475-15DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M90DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc