

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024695.D
 Acq On : 16 Feb 2022 14:39
 Operator : SY/MD
 Sample : N1475-16DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4M91DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	91	rBV	72081	71515	8.25%	1.444%
2	1.568	156	164	175	rBV	71994	81578	9.41%	1.648%
3	2.111	322	333	357	rVB	133366	196571	22.68%	3.970%
4	3.892	878	887	930	rBV2	46468	165114	19.05%	3.335%
5	4.349	1013	1029	1062	rBV	95207	241807	27.90%	4.883%
6	5.047	1229	1246	1273	rBV3	209758	520250	60.02%	10.507%
7	5.616	1412	1423	1449	rBV	133288	271675	31.34%	5.487%
8	5.912	1504	1515	1526	rBV5	4562	9396	1.08%	0.190%
9	6.069	1549	1564	1586	rBV	122932	249146	28.75%	5.032%
10	6.985	1838	1849	1876	rBV	57768	108382	12.50%	2.189%
11	7.317	1940	1952	1964	rBV	252343	440973	50.88%	8.906%
12	7.387	1964	1974	2006	rVB	503788	866730	100.00%	17.504%
13	7.622	2038	2047	2068	rBV2	32500	58838	6.79%	1.188%
14	8.088	2182	2192	2229	rBV	231830	451330	52.07%	9.115%
15	8.850	2419	2429	2461	rBV	221746	362491	41.82%	7.321%
16	10.214	2842	2853	2867	rBV	71927	114291	13.19%	2.308%
17	11.249	3162	3175	3192	rBV	236686	367805	42.44%	7.428%
18	11.622	3280	3291	3309	rBV	232468	361716	41.73%	7.305%
19	14.040	4031	4043	4053	rVB2	7506	11986	1.38%	0.242%




Sum of corrected areas: 4951594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024695.D
Acq On : 16 Feb 2022 14:39
Operator : SY/MD
Sample : N1475-16DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

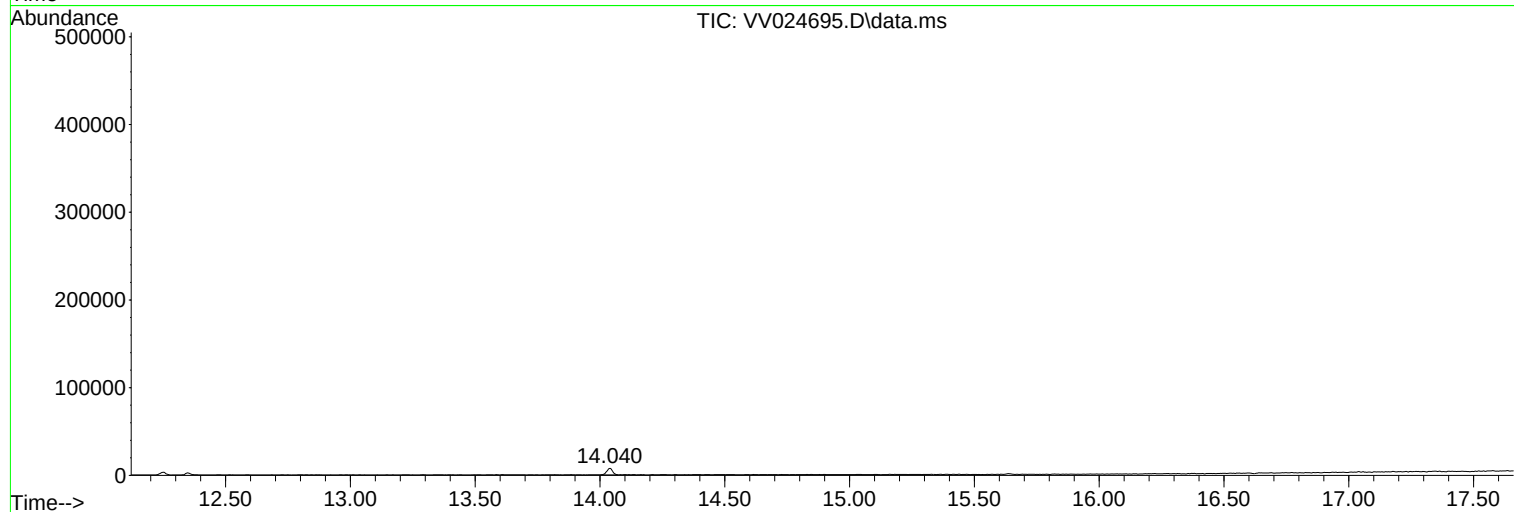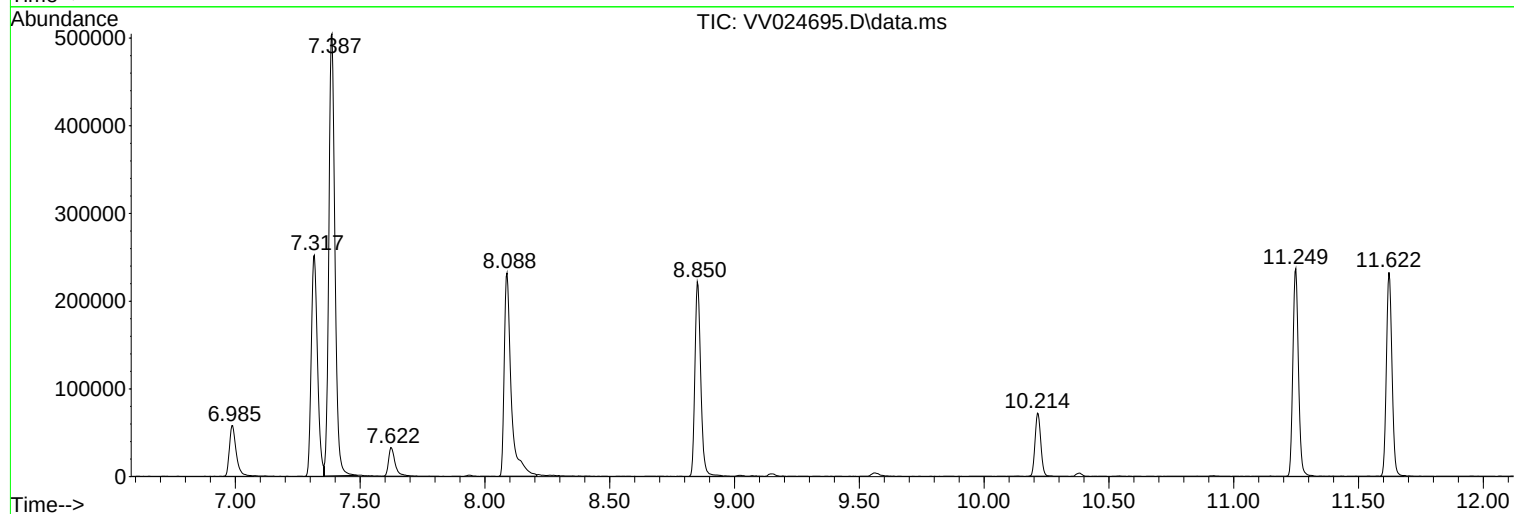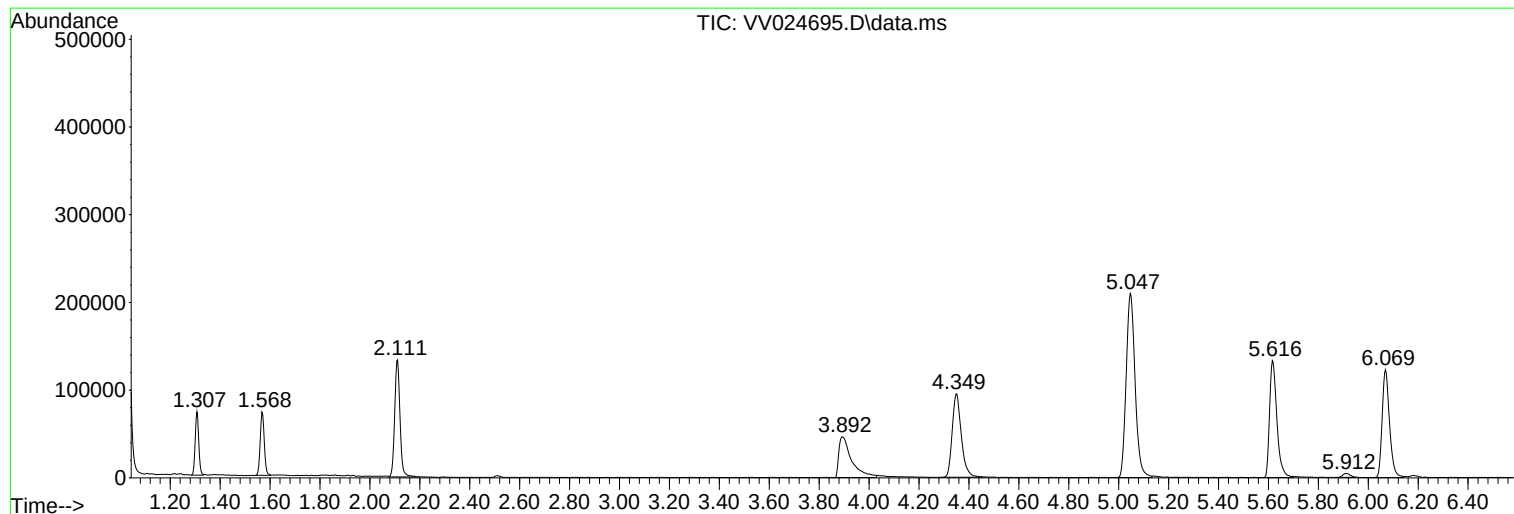

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024695.D
Acq On : 16 Feb 2022 14:39
Operator : SY/MD
Sample : N1475-16DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024695.D
Acq On : 16 Feb 2022 14:39
Operator : SY/MD
Sample : N1475-16DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4M91DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
