

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024696.D
 Acq On : 16 Feb 2022 15:07
 Operator : SY/MD
 Sample : N1475-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	109030	111254	18.30%	2.245%
2	1.571	157	165	178	rBV	90823	104032	17.12%	2.099%
3	2.111	319	333	358	rVB	183976	271554	44.68%	5.480%
4	2.507	448	456	468	rVB	5595	8683	1.43%	0.175%
5	3.896	878	888	918	rBV2	43921	153624	25.27%	3.100%
6	4.349	1012	1029	1064	rBV	101858	259644	42.72%	5.240%
7	5.047	1227	1246	1272	rBV2	245908	607826	100.00%	12.267%
8	5.616	1406	1423	1453	rBV	191308	390346	64.22%	7.878%
9	5.908	1505	1514	1531	rVB3	5683	12253	2.02%	0.247%
10	6.069	1551	1564	1593	rBV	135175	279722	46.02%	5.645%
11	6.985	1839	1849	1876	rBV2	65295	122136	20.09%	2.465%
12	7.313	1939	1951	1970	rBV	307085	534310	87.91%	10.783%
13	7.400	1972	1978	1985	rVB3	3632	6325	1.04%	0.128%
14	7.622	2038	2047	2070	rBV	35258	64097	10.55%	1.294%
15	8.088	2181	2192	2235	rBV	233168	465843	76.64%	9.401%
16	8.850	2418	2429	2457	rBV	311771	510423	83.98%	10.301%
17	10.214	2843	2853	2872	rBV	75868	119361	19.64%	2.409%
18	11.246	3163	3174	3198	rBV	341897	523920	86.20%	10.573%
19	11.622	3279	3291	3311	rBV	258747	409817	67.42%	8.270%




Sum of corrected areas: 4955170

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024696.D
Acq On : 16 Feb 2022 15:07
Operator : SY/MD
Sample : N1475-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

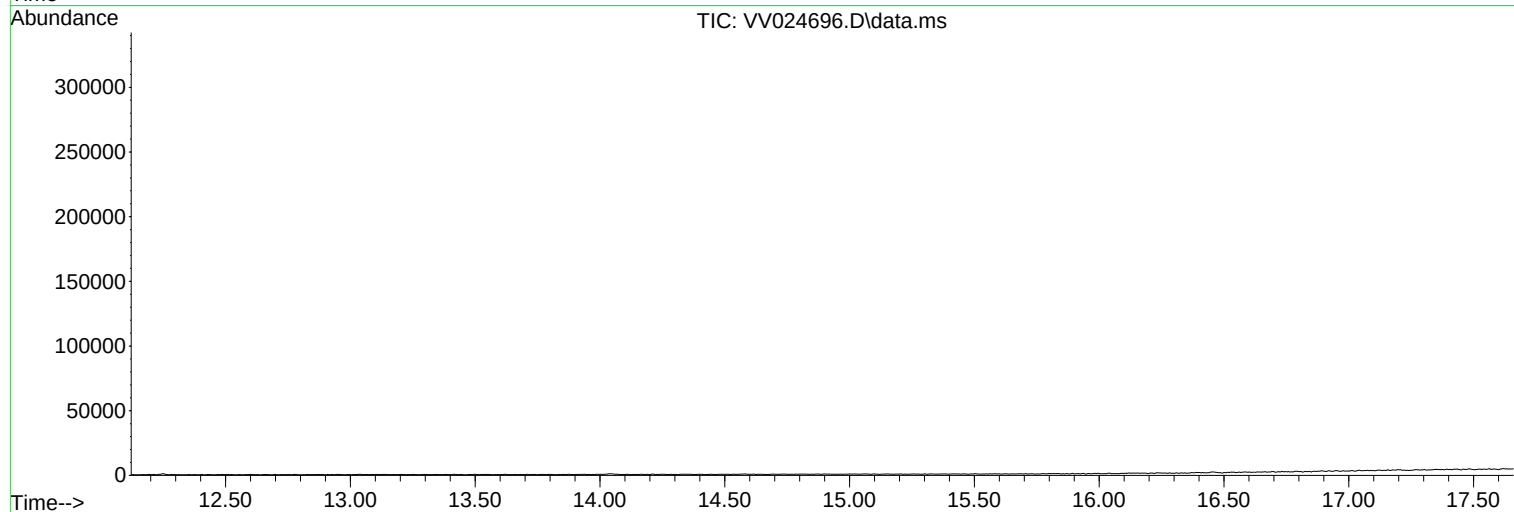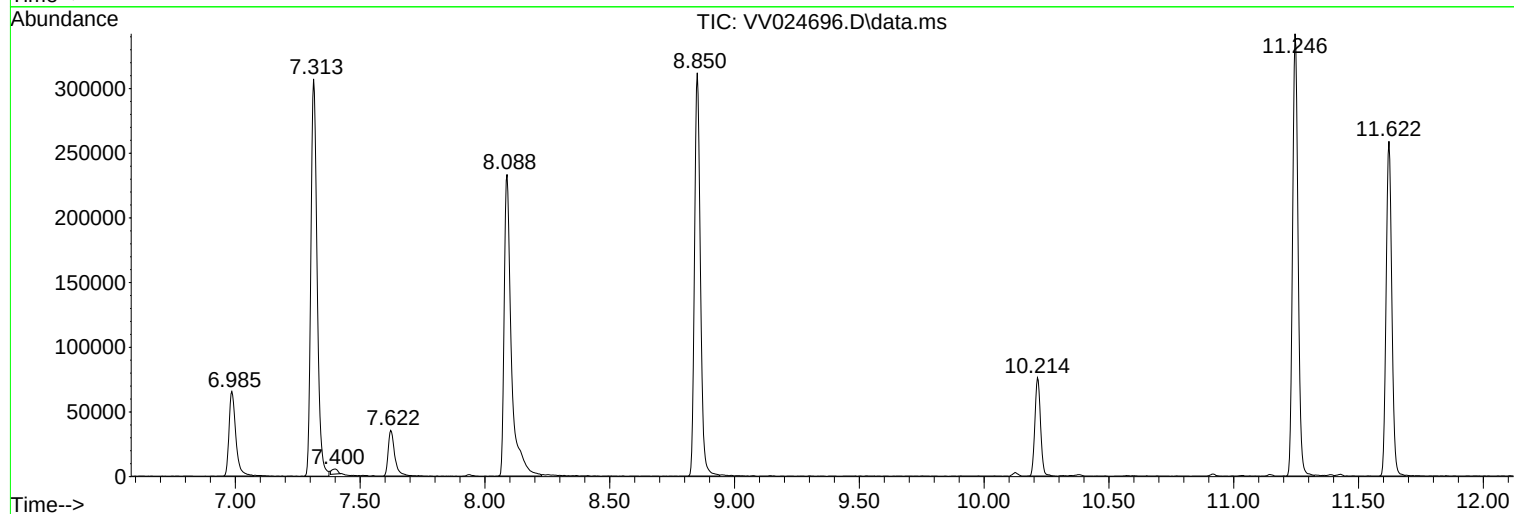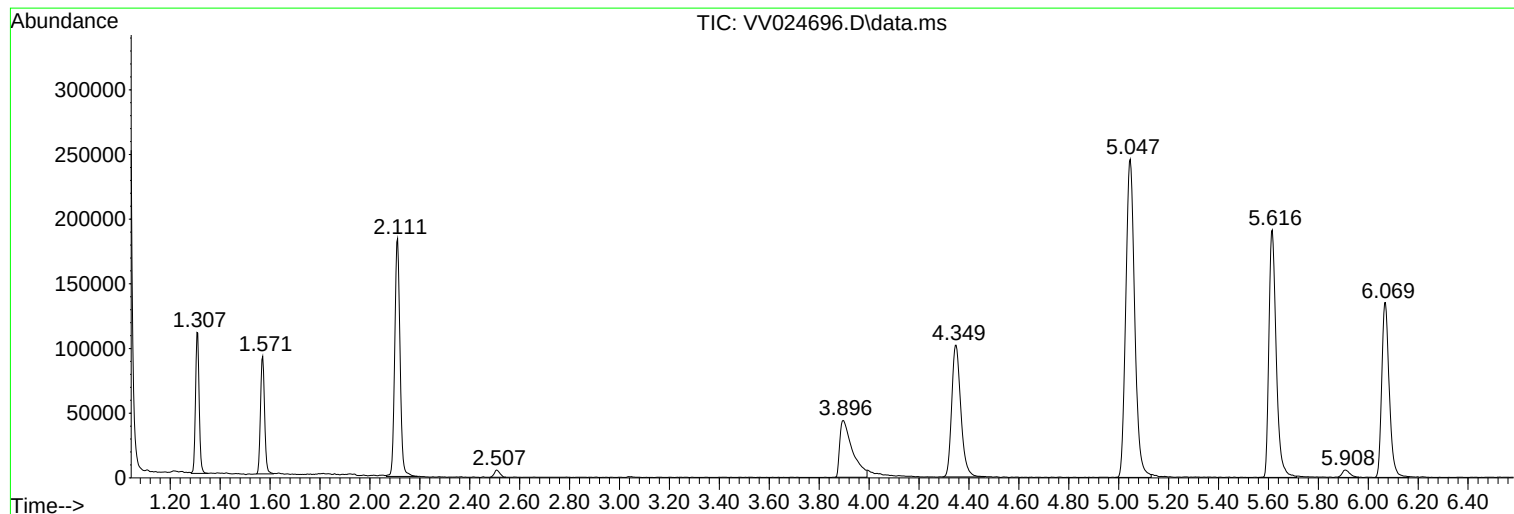

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024696.D
Acq On : 16 Feb 2022 15:07
Operator : SY/MD
Sample : N1475-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024696.D
Acq On : 16 Feb 2022 15:07
Operator : SY/MD
Sample : N1475-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc