

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
 Data File : VV024697.D
 Acq On : 16 Feb 2022 15:30
 Operator : SY/MD
 Sample : N1480-12DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCX8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	71481	74595	9.65%	1.418%
2	1.571	157	165	176	rBV	74644	85089	11.00%	1.617%
3	2.111	323	333	354	rVB	136317	201064	26.00%	3.822%
4	3.899	879	889	922	rBV2	46602	162771	21.05%	3.094%
5	4.352	1014	1030	1056	rBV2	95317	240378	31.08%	4.569%
6	5.050	1231	1247	1278	rBV2	218962	552374	71.43%	10.500%
7	5.619	1411	1424	1457	rBV	167428	340312	44.01%	6.469%
8	5.915	1502	1516	1530	rBV6	4785	9591	1.24%	0.182%
9	6.069	1552	1564	1598	rBV	125178	266136	34.42%	5.059%
10	6.989	1839	1850	1872	rBV	58215	109783	14.20%	2.087%
11	7.317	1941	1952	1971	rBV	258976	451042	58.33%	8.574%
12	7.625	2038	2048	2066	rBV	32600	59326	7.67%	1.128%
13	8.088	2182	2192	2230	rBV	235350	463890	59.99%	8.818%
14	8.854	2418	2430	2432	rBV	299777	389664	50.39%	7.407%
15	8.879	2433	2438	2471	rVB	479804	773307	100.00%	14.700%
16	10.214	2842	2853	2871	rBV	76971	120069	15.53%	2.282%
17	11.246	3164	3174	3196	rVV	302913	504667	65.26%	9.593%
18	11.622	3278	3291	3310	rBV	242838	390042	50.44%	7.414%
19	12.249	3476	3486	3496	rBV2	7914	12486	1.61%	0.237%
20	14.040	4032	4043	4052	rBV2	8338	13685	1.77%	0.260%
21	15.503	4488	4498	4509	rBV2	27155	40384	5.22%	0.768%




Sum of corrected areas: 5260655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024697.D
Acq On : 16 Feb 2022 15:30
Operator : SY/MD
Sample : N1480-12DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

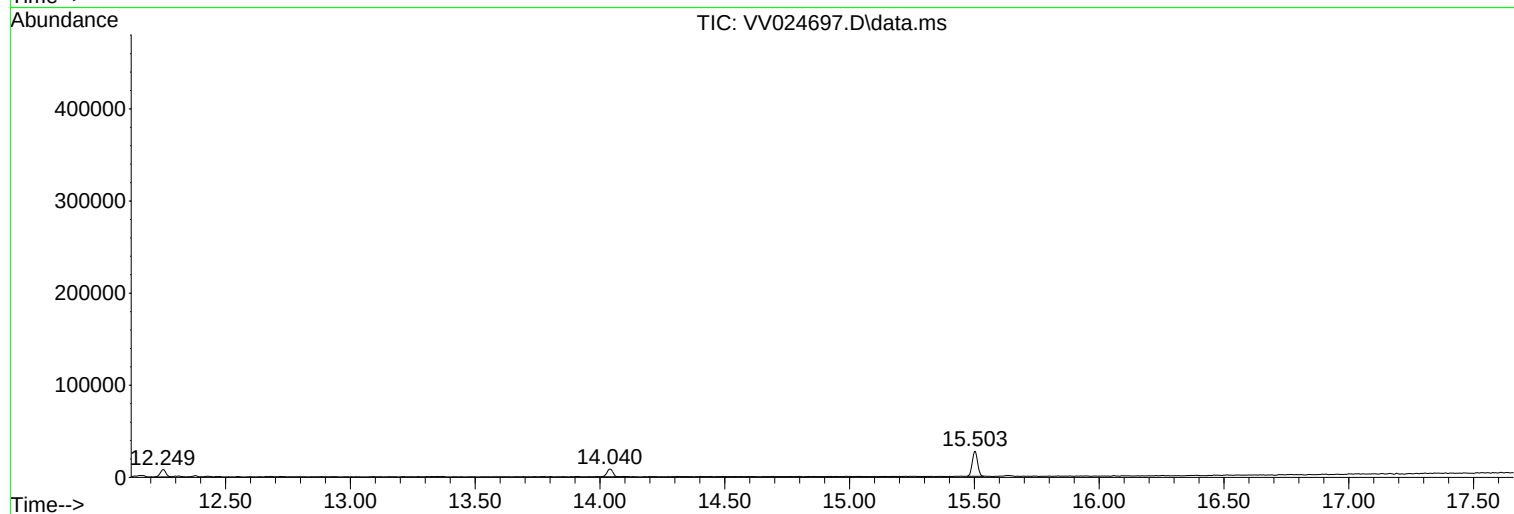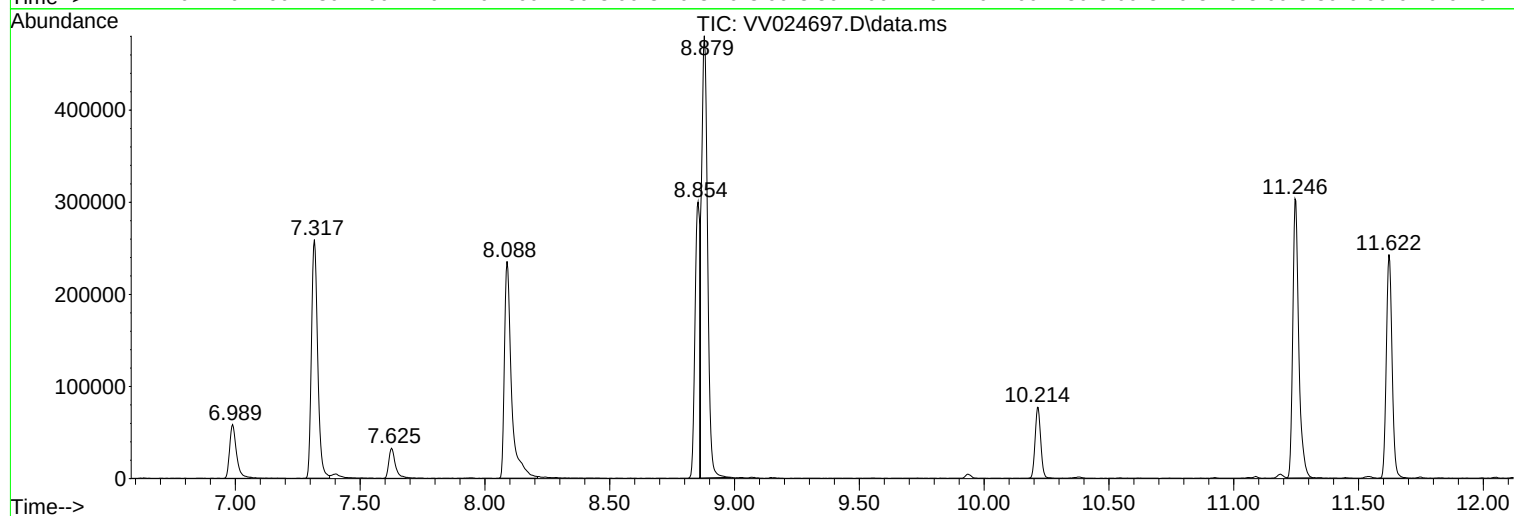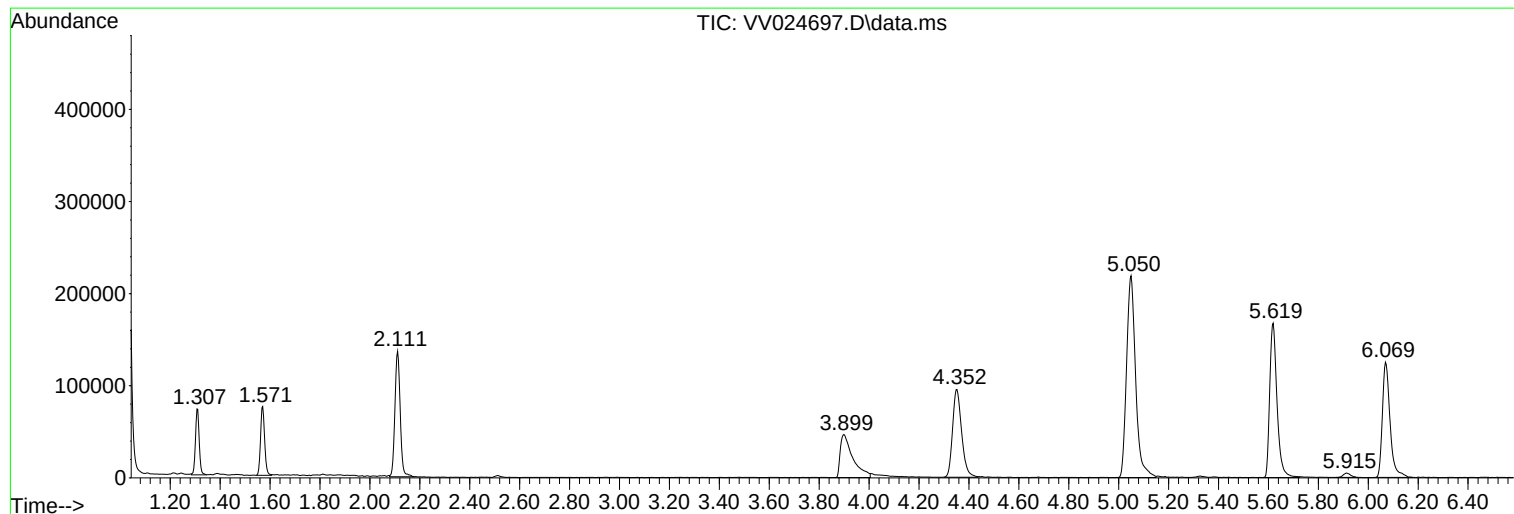

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024697.D
Acq On : 16 Feb 2022 15:30
Operator : SY/MD
Sample : N1480-12DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021622\
Data File : VV024697.D
Acq On : 16 Feb 2022 15:30
Operator : SY/MD
Sample : N1480-12DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc